


U.S. ARMY TANK AUTOMOTIVE RESEARCH, DEVELOPMENT AND ENGINEERING CENTER (TARDEC)



Army Demonstration of Light Obscuration Particle Counters for Monitoring Aviation Fuel Contamination

Joel Schmitigal, Jill Bramer
Chemists, TARDEC

7 May 2013

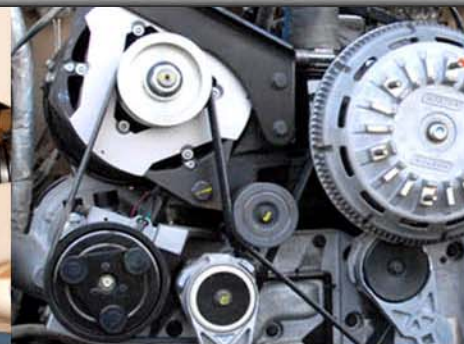

Report Documentation Page				Form Approved OMB No. 0704-0188	
Public reporting burden for the collection of information is estimated to average 1 hour per response, including the time for reviewing instructions, searching existing data sources, gathering and maintaining the data needed, and completing and reviewing the collection of information. Send comments regarding this burden estimate or any other aspect of this collection of information, including suggestions for reducing this burden, to Washington Headquarters Services, Directorate for Information Operations and Reports, 1215 Jefferson Davis Highway, Suite 1204, Arlington VA 22202-4302. Respondents should be aware that notwithstanding any other provision of law, no person shall be subject to a penalty for failing to comply with a collection of information if it does not display a currently valid OMB control number.					
1. REPORT DATE 07 AUG 2013		2. REPORT TYPE Briefing Charts		3. DATES COVERED 01-08-2013 to 04-08-2013	
4. TITLE AND SUBTITLE Army Demonstration of Light Obscuration Particle Counters for Monitoring Aviation Fuel Contamination				5a. CONTRACT NUMBER	
				5b. GRANT NUMBER	
				5c. PROGRAM ELEMENT NUMBER	
6. AUTHOR(S) Joel Schmitigal; Jill Bramer				5d. PROJECT NUMBER	
				5e. TASK NUMBER	
				5f. WORK UNIT NUMBER	
7. PERFORMING ORGANIZATION NAME(S) AND ADDRESS(ES) U.S. Army TARDEC, 6501 East Eleven Mile Rd, Warren, Mi, 48397-5000				8. PERFORMING ORGANIZATION REPORT NUMBER #24085	
9. SPONSORING/MONITORING AGENCY NAME(S) AND ADDRESS(ES) U.S. Army TARDEC, 6501 East Eleven Mile Rd, Warren, Mi, 48397-5000				10. SPONSOR/MONITOR'S ACRONYM(S) TARDEC	
				11. SPONSOR/MONITOR'S REPORT NUMBER(S) #24085	
12. DISTRIBUTION/AVAILABILITY STATEMENT Approved for public release; distribution unlimited					
13. SUPPLEMENTARY NOTES					
14. ABSTRACT briefing charts					
15. SUBJECT TERMS					
16. SECURITY CLASSIFICATION OF:			17. LIMITATION OF ABSTRACT Public Release	18. NUMBER OF PAGES 66	19a. NAME OF RESPONSIBLE PERSON
a. REPORT unclassified	b. ABSTRACT unclassified	c. THIS PAGE unclassified			



Project Background

Unclassified



- Evaluation of In-line and Laboratory Particle Counters for US Military applications:
 - AFCTK/PTK
 - PQAS-E
 - Online fuel contamination monitoring
- Tri-Service project funded by DLA-Energy
 - Army received \$45,000
- Complimentary testing to programs completed by the Energy Institute, Navy, TFLRF, and Parker Hannifin



Project Background – Current Methods

Unclassified



Current methods:

- ASTM D2276 – Particulate Contamination in Aviation Fuel by Line Sampling
- ASTM D3240 – Undissolved Water in Aviation Turbine Fuels
- ASTM D4176 – Free Water and Particulate Contamination in Distillate Fuels (Visual Inspection Procedures)

Drawbacks:

- Operator Subjectivity
- Large sample volumes
- Potential Contamination



DEF STAN 91-91 and MIL-DTL-83133 both include a report only requirement for particle counting

- IP 564 – Parker ACM20
- IP 565/ASTM D7619 – Stanhope-Seta AvCount
- IP 577 – Pamas S40
- Parker icountOS - Online instrument

Drawbacks to electronic methods

- Unable to distinguish between free water, sediment, and air bubbles



Objective

Unclassified



- Utilize existing particle counter technology to monitor aviation fuel quality for 5 days at 2 Army sites.
- Monitor fixed and mobile infrastructure points used to receive, store, and distribute aviation turbine fuel.
- Near real-time and laboratory non-subjective data analysis of the quality of aviation turbine fuel compared to military and industry accepted methods.



Electronic Sensor History



Unclassified

- Particle counting is not a new science
- Hydraulic industry has utilized this technology for decades and created a mature process
- Hydraulic industry has developed recognized calibration methodologies and standardized cleanliness code ratings
 - ISO 11171
 - ISO 4406
- Challenge – Being able to determine both particulate and water contamination

ISO/Range Code	Min. particles /mL	Max particles /mL
1	0	0.02
2	0.02	0.04
3	0.04	0.08
4	0.08	0.15
5	0.15	0.3
6	0.3	0.6
7	0.6	1.3
8	1.3	2.5
9	2.5	5
10	5	10
11	10	20
12	20	40
13	40	80
14	80	160
15	160	320
16	320	640
17	640	1,300
18	1,300	2,500
19	2,500	5,000
20	5,000	10,000
21	10,000	20,000
22	20,000	40,000
23	40,000	80,000
24	80,000	160,000
25	160,000	320,000
26	320,000	640,000
27	640,000	1,300,000
28	1,300,000	2,500,000
29	2,500,000	5,000,000
30	5,000,000	10,000,000



Proposed Particle Count Limits



Unclassified

	Receipt	Vehicle Fuel Tank	Fuel Injector
Aviation Fuel			
DEF (AUST) 5695B		18/16/13	
Parker	18/16/13	14/10/7	
Pamas/Parker/Particle Solutions	19/17/12		
U.S. Army	19/17/14/13*		
Diesel Fuel			
World Wide Fuel Charter 4th		18/16/13	
DEF (AUST) 5695B		18/16/13	
Bosch/Cummins		18/16/13	
Donaldson	22/21/18	14/13/11	12/9/6
Pall	17/15/12	15/14/11	12/9/6 11/8/7

* 4um (c)/ 6um (c)/ 14um (c)/ 30um (c)



Evaluation Details



Unclassified

Two types of instruments

Online



Lab-based






Site I – Fuel Distribution



Unclassified

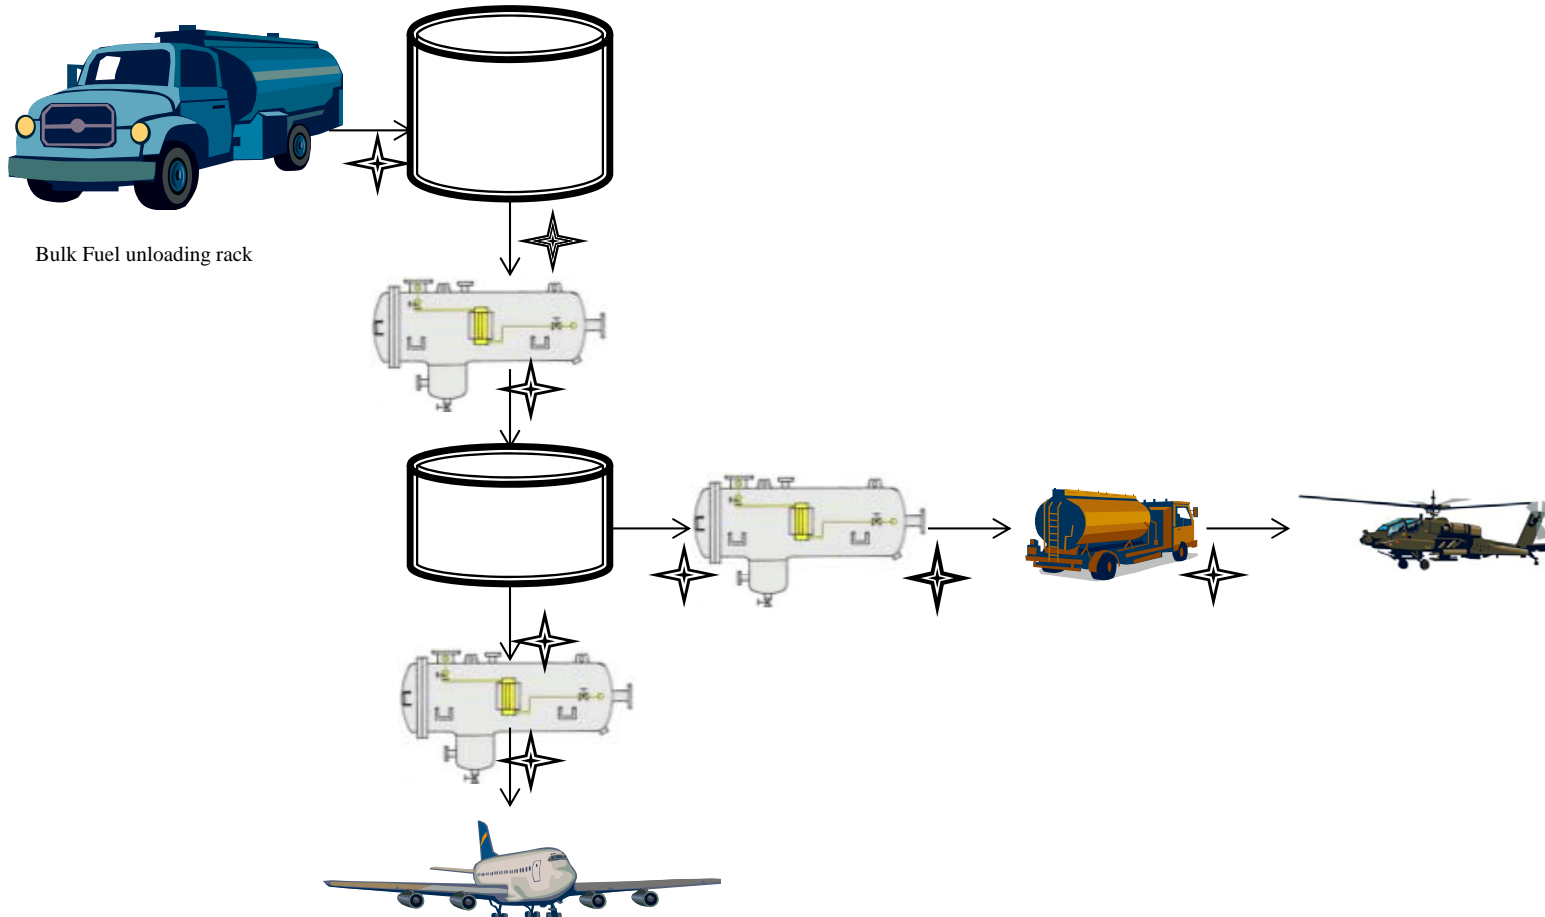

Fuel sampling points



Site I – Bulk Delivery Offload



Unclassified





Site I – Bulk Sampling



Unclassified



- Matched Weight Monitor Samples
- Aqua-Glo Sample (1L)
- 1-gallon sample for lab instruments



U.S. ARMY
RDECOM
RESEARCH DEVELOPMENT ENGINEERING CENTER

Site I – Bulk Sampling

Unclassified



Online instruments


- Parker Hannifin icountOS
- Measuring particles in fuel flow from truck to bulk storage tank.
- Instrument averages 2 minutes of data.
- For our application, we manually started the pump.



Bulk Day 1



Unclassified

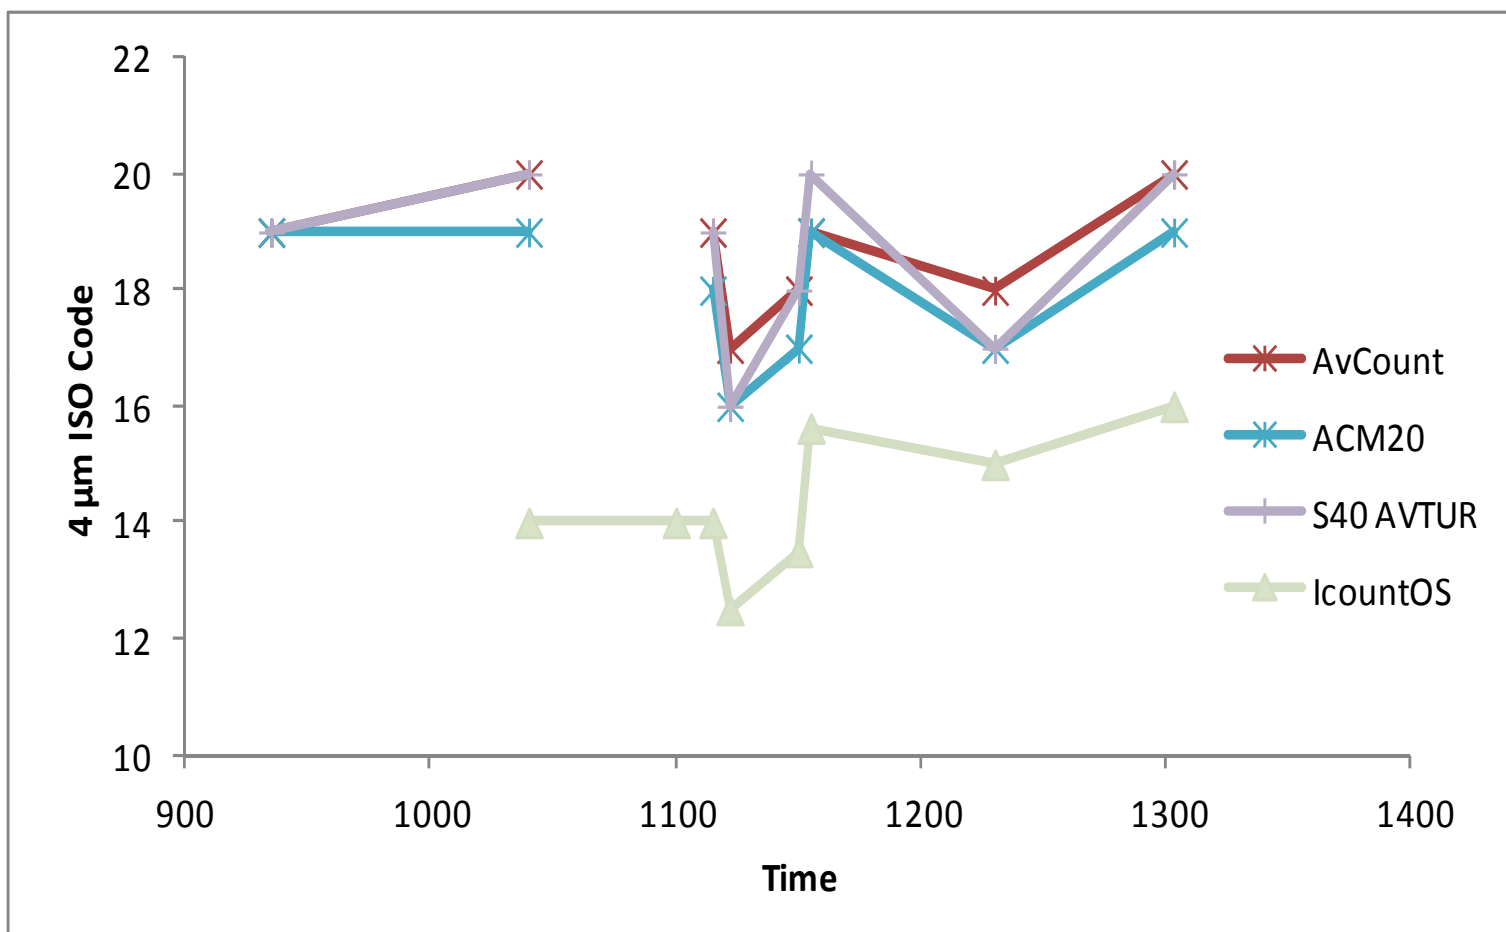



Sample can contamination

Unclassified






Bulk Day 2



Unclassified

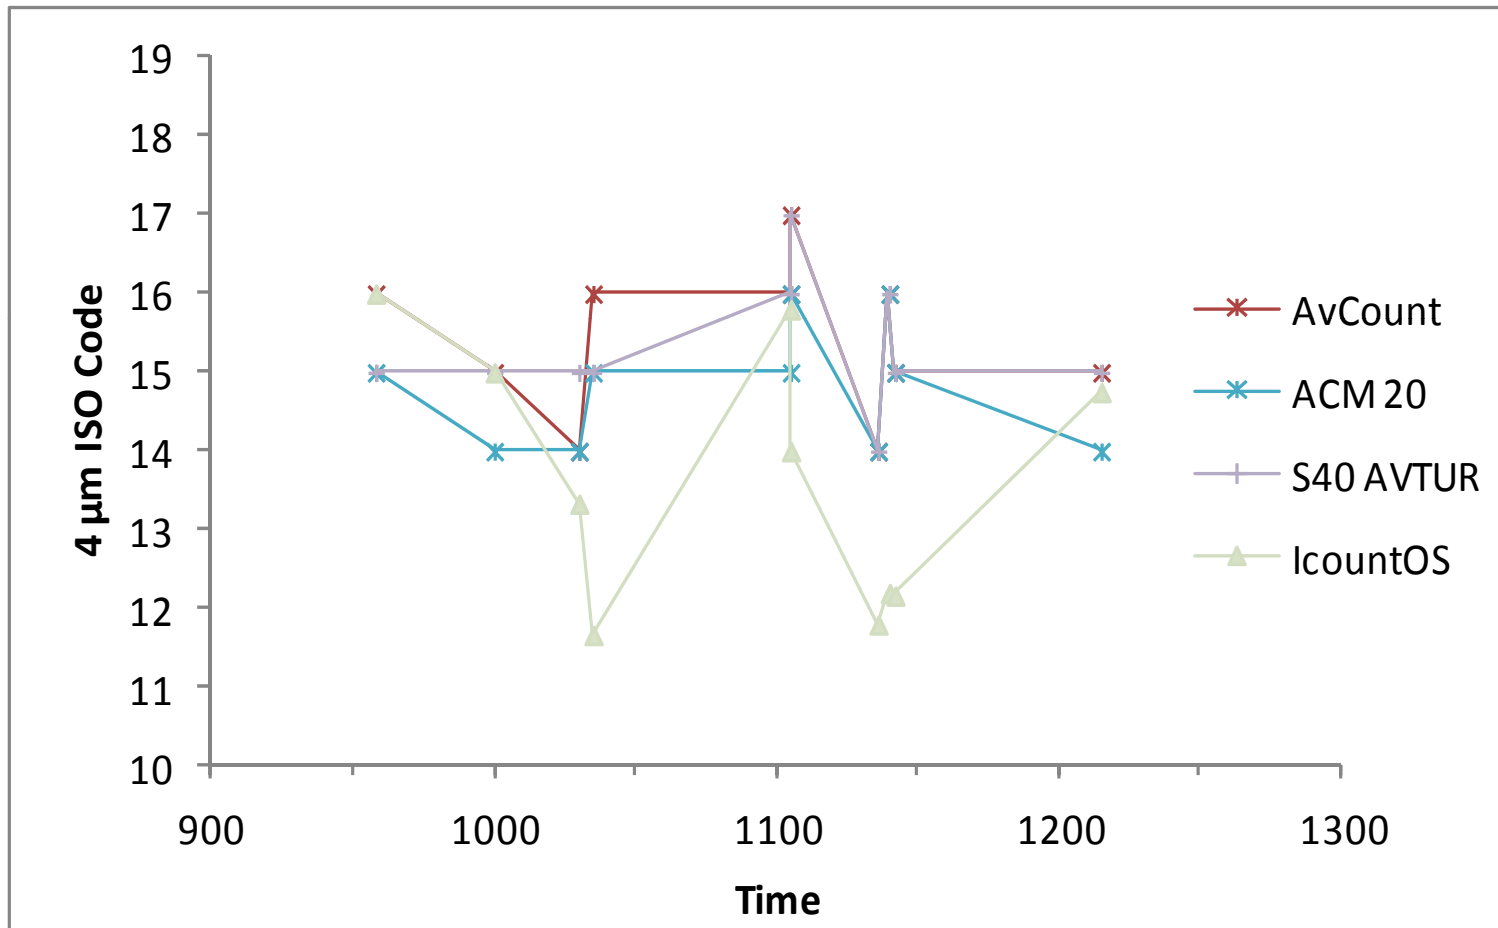



U.S. ARMY
RDECOM
RESEARCH DEVELOPMENT ENGINEERING CENTER

Site I – Transfer from Bulk Storage



Unclassified




- Samples taken upstream and downstream of the Filter Separator



Site I – Transfer from Bulk Storage 4 micron



Unclassified

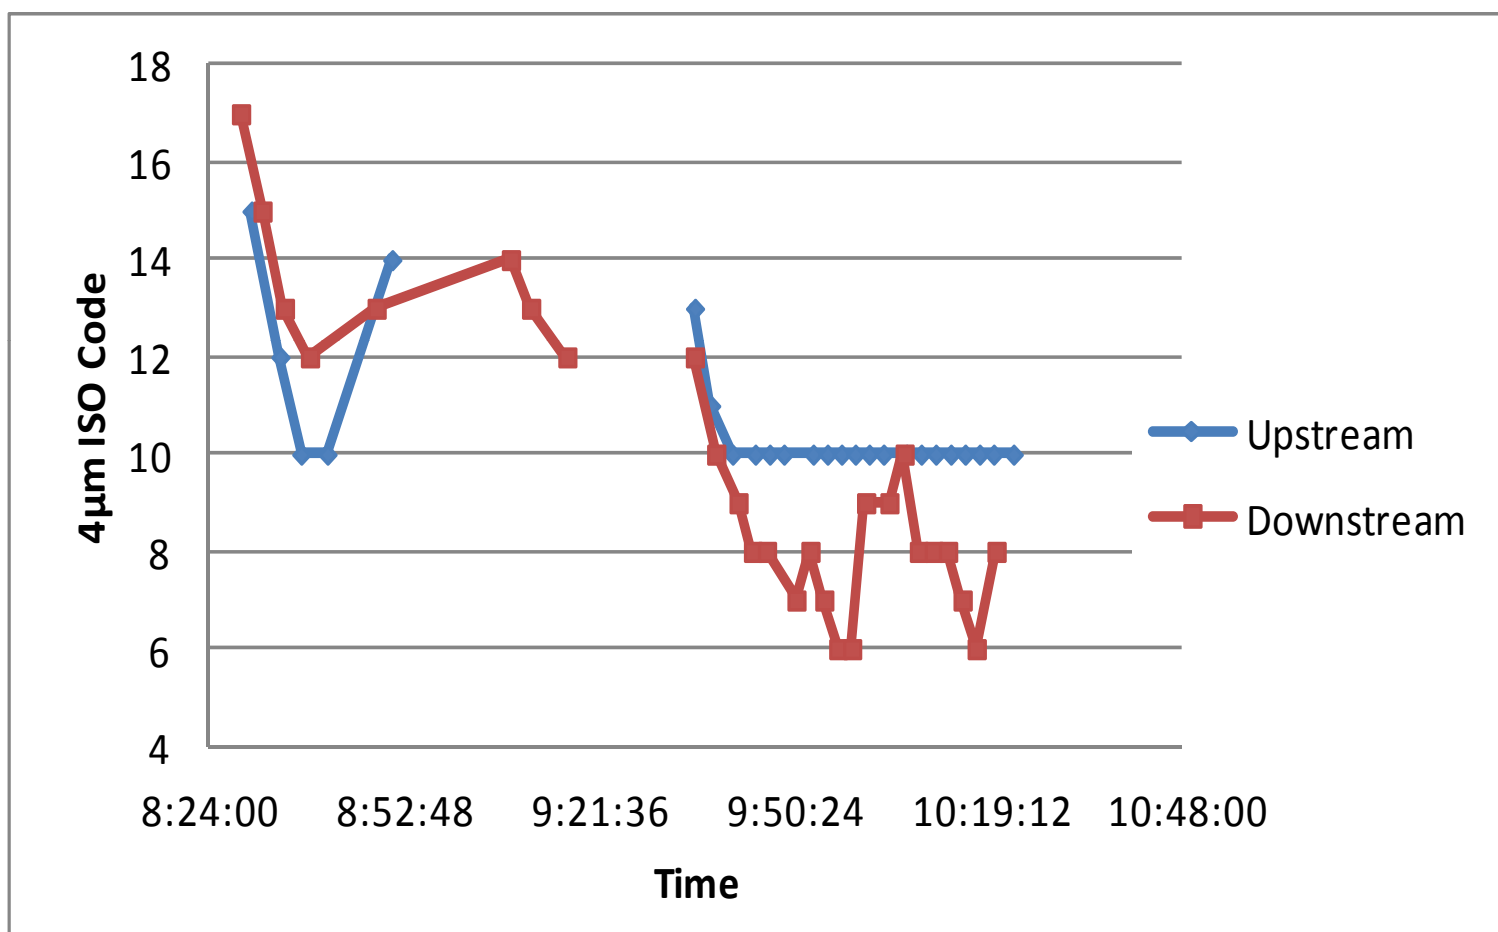




Site I – Transfer from Bulk Storage 6 micron



Unclassified

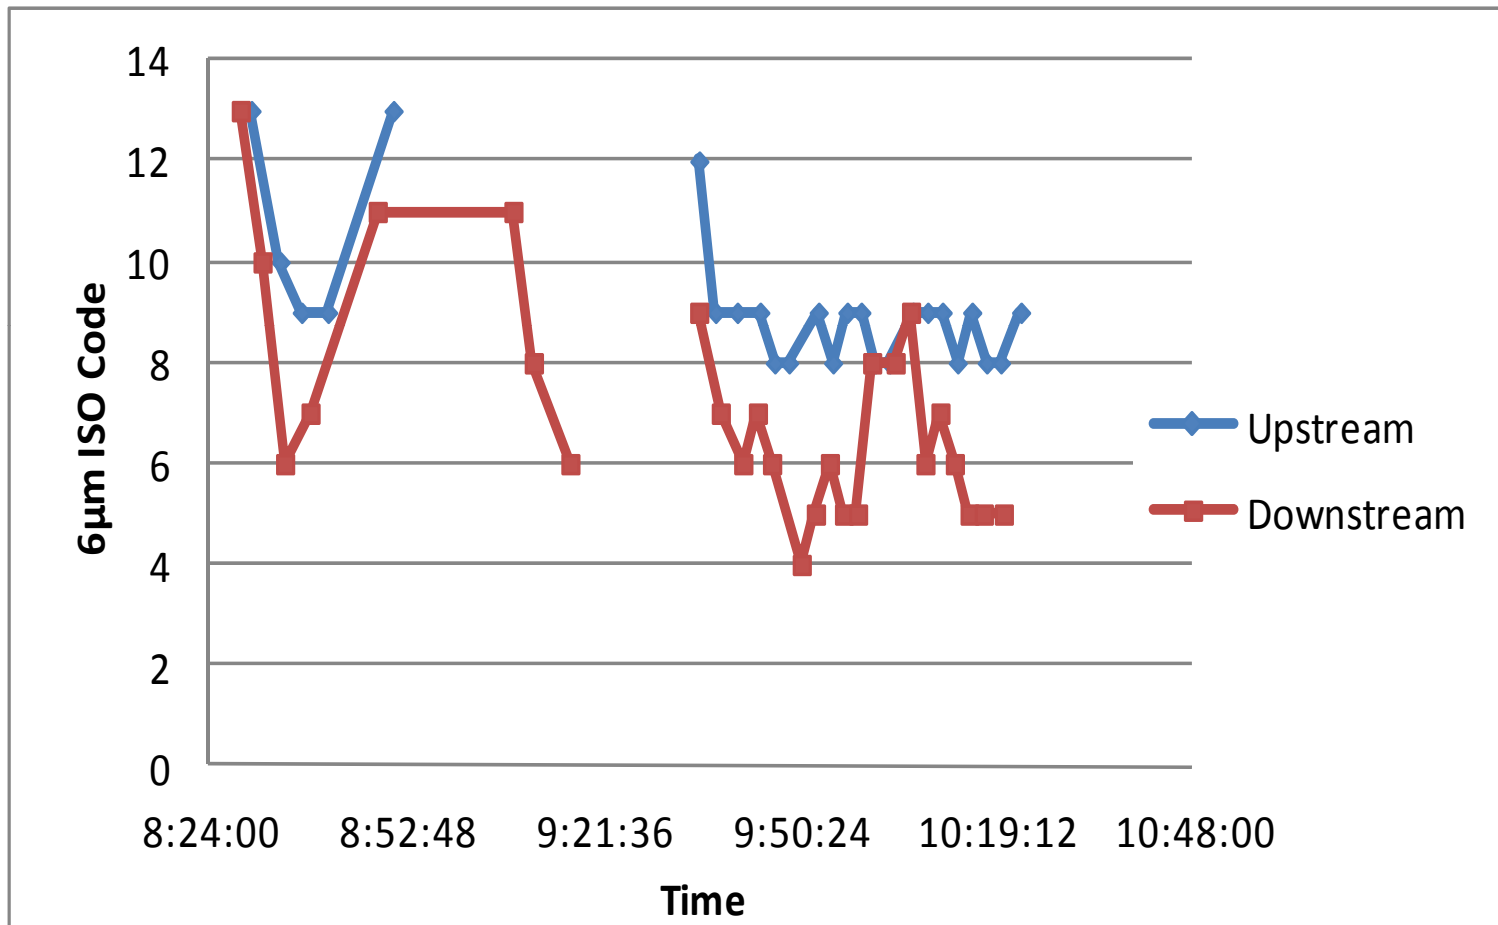




Site I – Transfer from Bulk Storage 14 micron



Unclassified

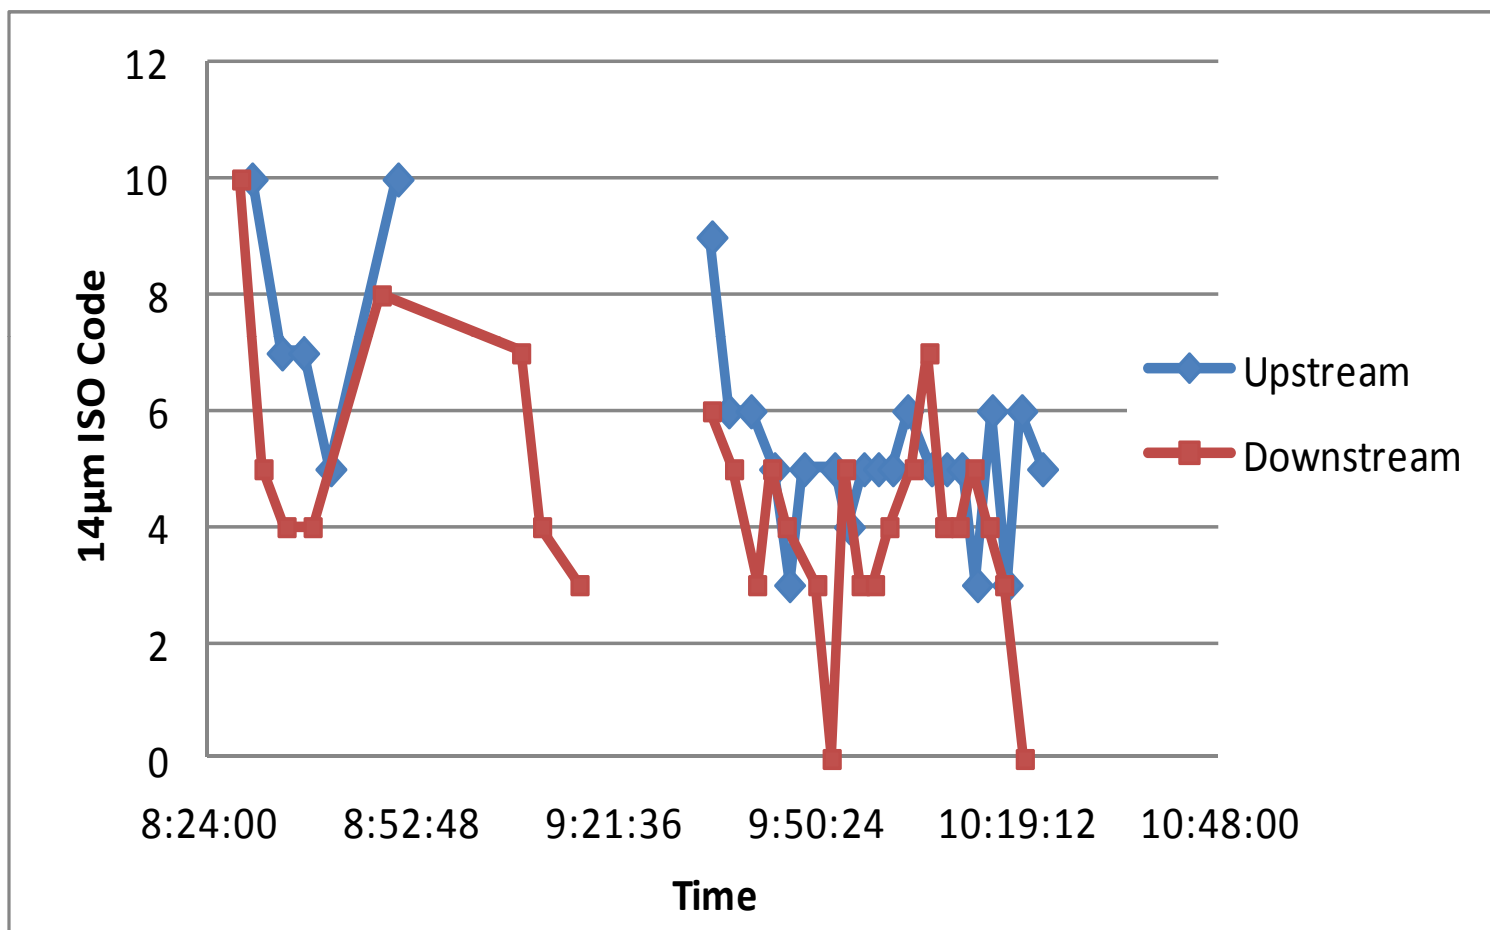



Site I – Transfer from Bulk Storage



Unclassified

Time (EST)	mg/L	Location	Lab ID	Avcount	ACM20 #1	ACM20 #2	S40 AVTUR #1	S40 AVTUR #2
830	1.11	Upstream	22	14/13/9/5	13/12/8/4	14/12/8/5	14/12/9/-	14/12/8/-
			22A	15/13/10/6	14/12/8/5	14/12/9/5	14/13/9/-	15/13/9/-
830	1.33	Downstream	23	14/12/9/4	13/12/8/4	14/12/9/5	14/12/9/-	14/12/9/-
			23A	15/13/10/7	14/12/9/5	14/12/9/5	15/13/10/-	15/13/9/-
918	0.60	Upstream	24	15/13/10/7	14/12/9/4	14/12/9/4	15/13/10/-	15/13/10/-
			24A	15/14/10/6	15/13/9/4	15/13/9/5	15/14/10/-	15/13/10/-
918	1.25	Downstream	25	15/13/9/5	14/12/8/4	14/12/8/4	14/13/9/-	14/12/9/-
			25A	16/14/11/7	15/13/8/7	15/13/10/6	15/14/10/-	15/14/10/-
1030	0.00	Upstream	26	14/12/9/5	14/12/8/0	14/12/8/4	14/12/9/-	15/12/9/-
			26A	15/13/10/6	14/13/9/4	14/13/9/5	15/13/10/-	15/13/10/-
1030	2.00*	Downstream	27	16/13/9/5	15/12/8/5	15/12/8/4	15/12/8/-	15/12/9/-
			27A	16/14/10/6	15/13/9/5	15/13/9/5	16/13/10/-	16/13/10/-



Site I – Fuel Dispensing

Unclassified



Dispensing Station for Refueling Trucks



Site I – Dispensing



Unclassified

Date	Time (EST)	mg/L	Location	Lab ID	Avcount	ACM20 #1	ACM20 #2	S40 AVTUR #1	S40 AVTUR #2	IOS
9 Apr 2013	1310	1.13	Upstream	20	16/14/11/7	15/14/10/6	15/14/10/5	16/14/11/-	16/14/11/-	12/10/7/3
				20A	16/15/11/7	16/14/10/7	16/14/10/7	16/14/11/-	16/14/11/-	
	1310	0.40	Downstream	19	18/16/12/8	17/15/11/7	17/15/11/6	17/15/12/-	17/15/12/-	13/11/8/6
				19A	18/16/12/8	17/15/11/7	17/15/11/7	17/16/12/-	17/15/12/-	
	1330	0.30	Truck	21	15/14/11/7	15/13/9/5	15/13/10/6	15/14/10/-	15/14/10/-	10/8/5/2
			Downstream	21A	16/14/11/7	15/14/10/6	15/14/10/5	16/14/11/-	16/14/11/-	
10 Apr 2013	1324	0.38	Upstream	29	16/14/11/7	15/13/10/5	15/13/10/6	15/13/10/-	15/13/11/-	
				29A	16/14/11/8	15/14/10/7	15/14/10/6	16/14/11/-	16/14/11/-	
	1324	0.00	Downstream	28	17/15/11/7	16/14/10/5	16/14/10/6	17/14/11/-	17/15/11/-	
				28A	17/15/11/7	17/14/10/7	17/14/10/7	17/15/11/-	17/15/11/-	
	1115	-	Truck Downstream	-						11/8/6/0



Site I – Fuel Dispensing



Unclassified

- Dispensing from COCO Refueling Truck into HEMTT (~4700 gallons)






Site I – Dispensing C5 Refueling



Unclassified

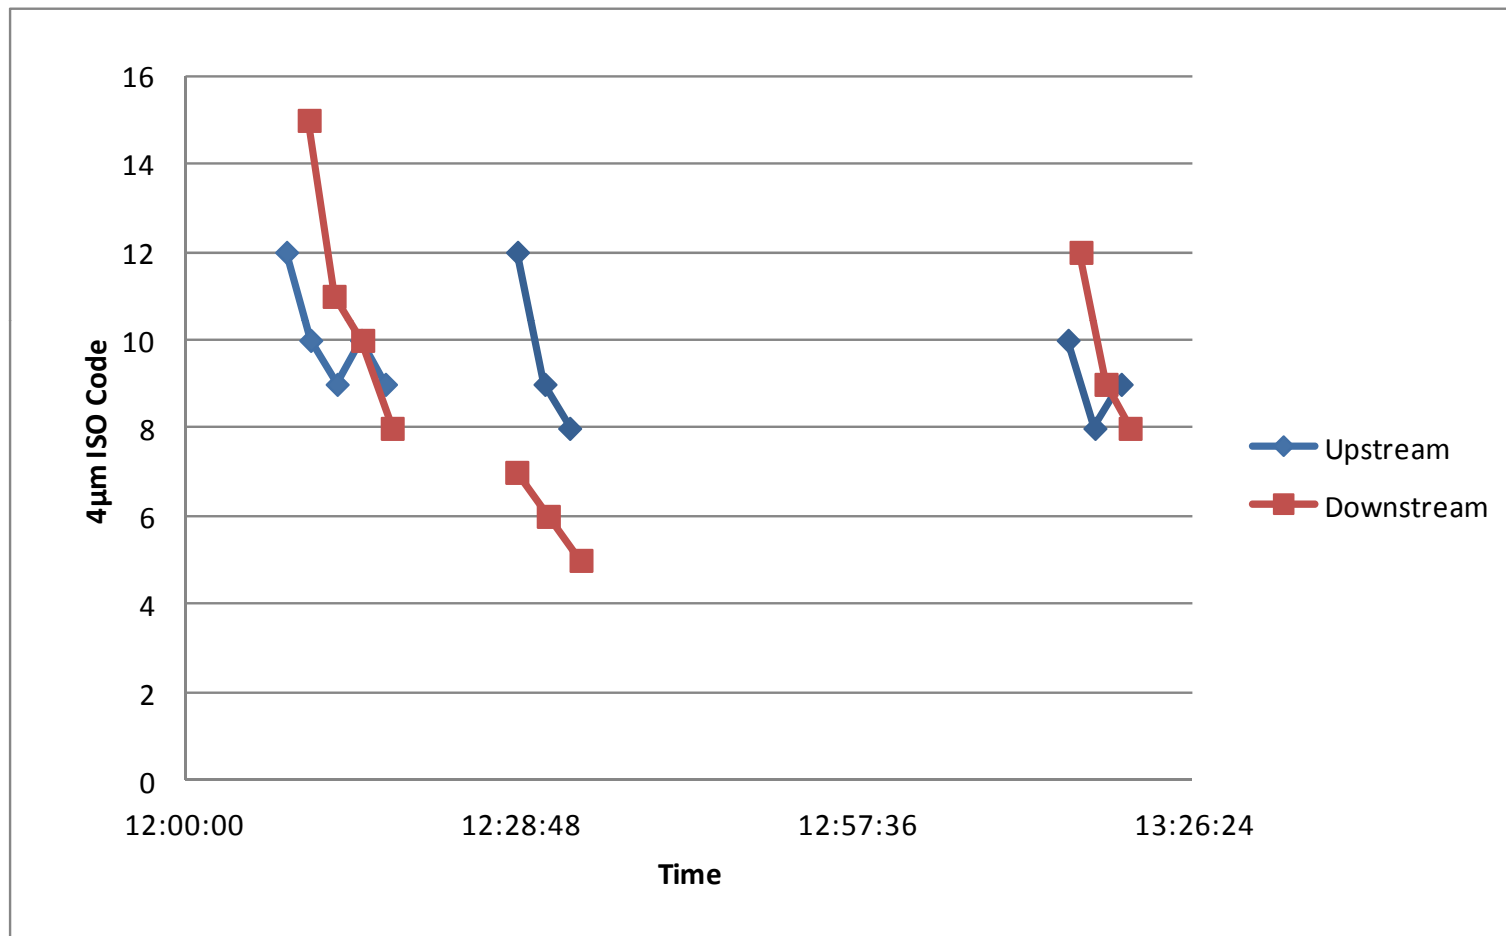




Site I – Dispensing C5 Refueling



Unclassified

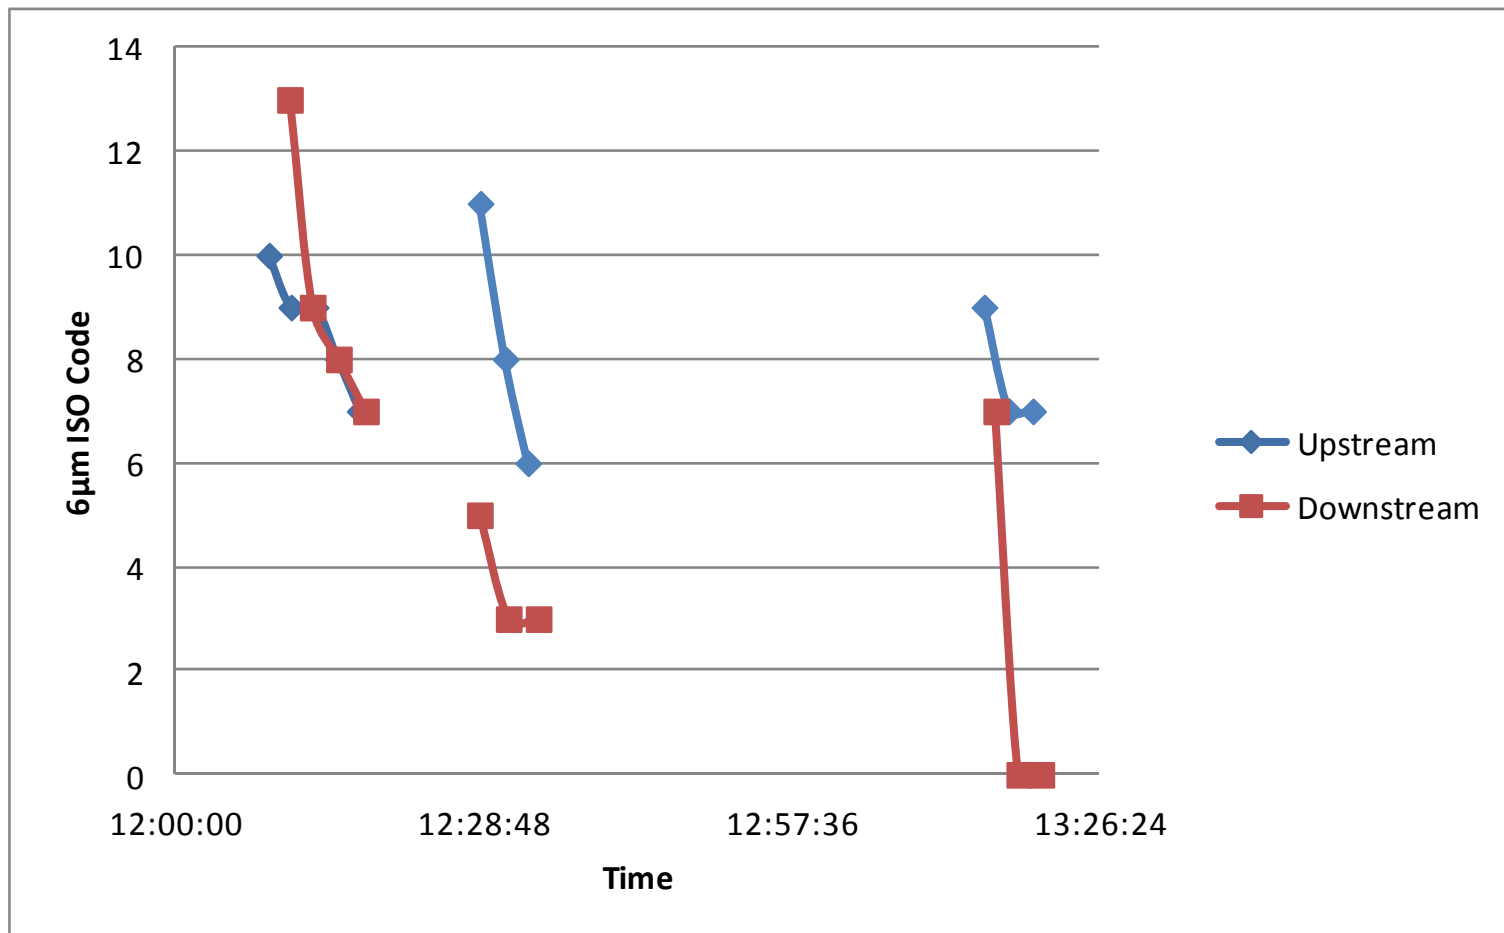




Site I – Dispensing C5 Refueling



Unclassified

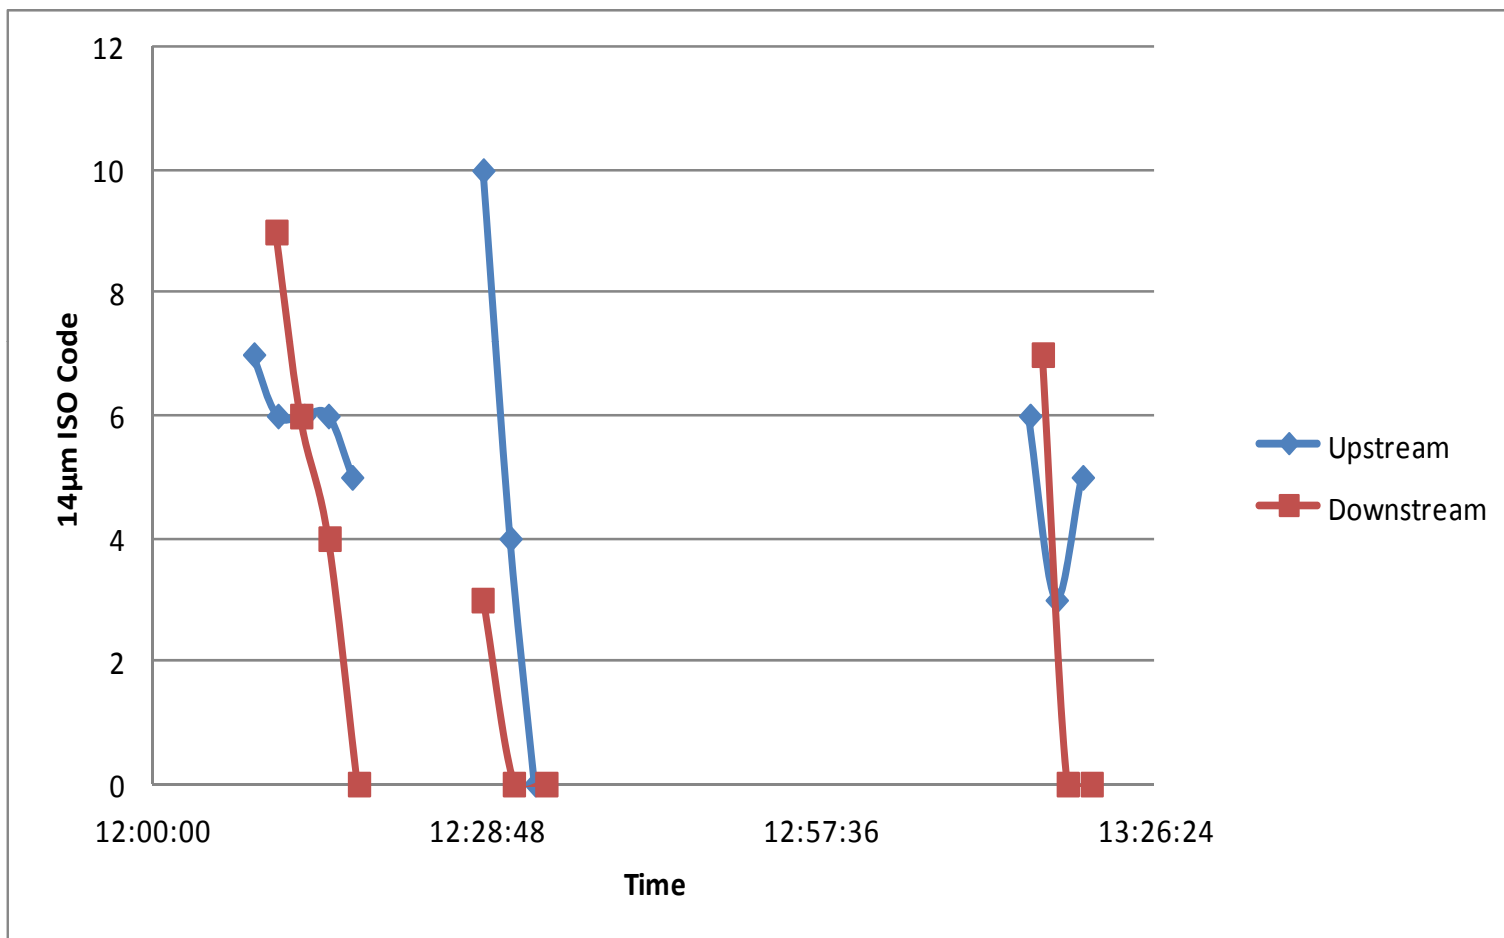




Site I – C17 Refueling



Unclassified

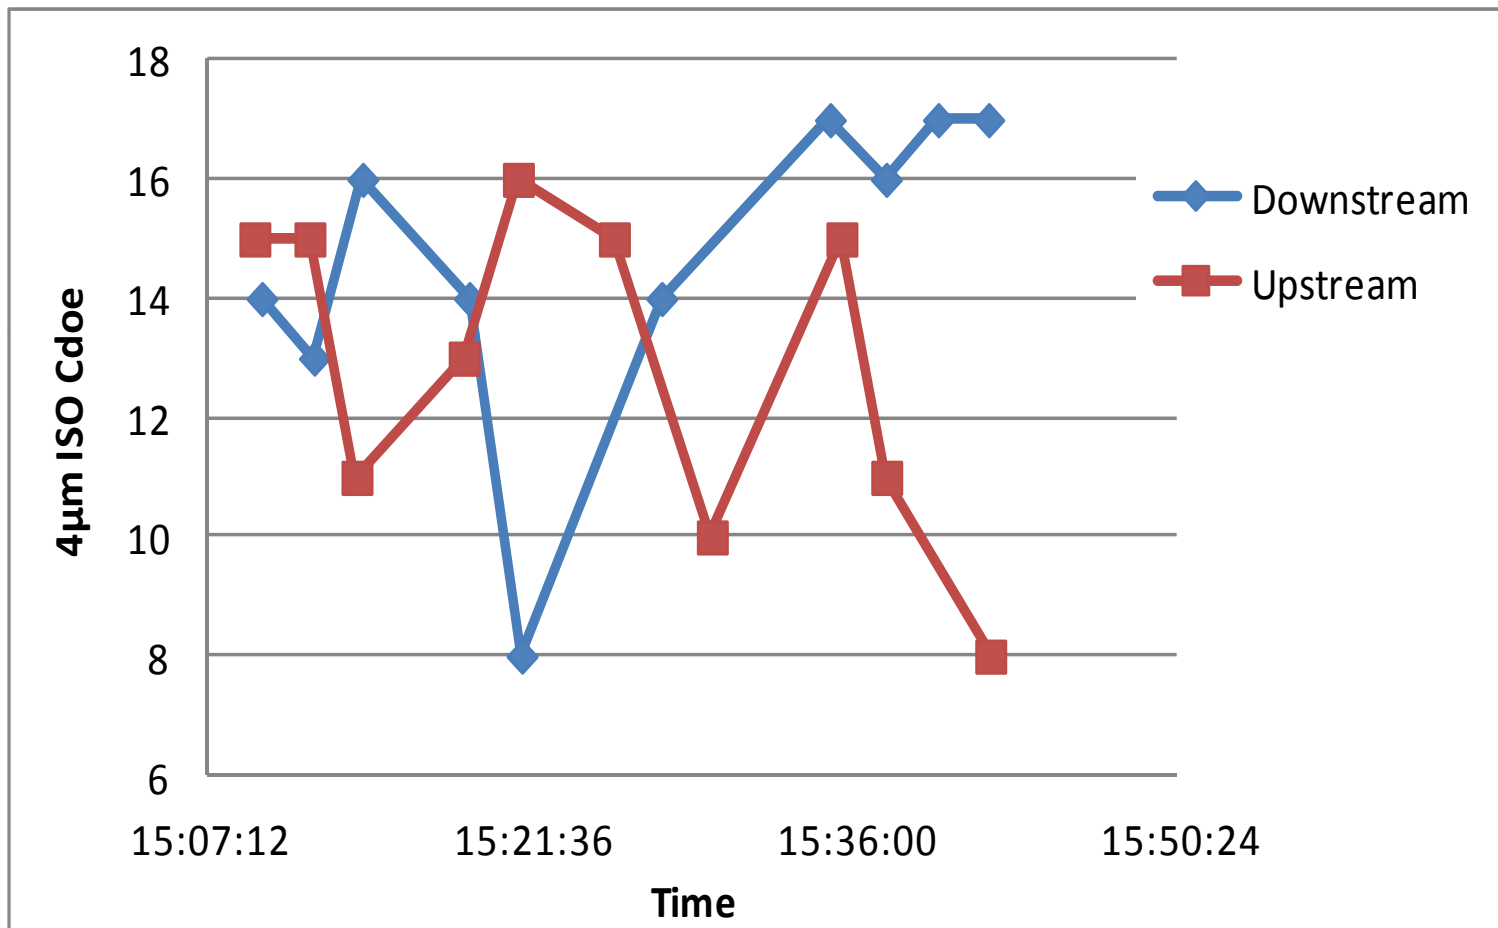



Site I – C17 Refueling



Unclassified

Time (EST)	mg/L	Location	Lab ID	Avcount	ACM-20 #1	ACM-20 #2	S40 AVTUR #1	S40 AVTUR #2
1511	0.70	Upstream	31	16/14/10/7	16/13/10/7	16/13/10/6	16/14/10/-	16/14/10/-
			31A	17/14/11/7	16/14/10/6	16/14/10/6	16/14/11/-	16/14/10/-
1511	0.25	Downstream	30	16/14/11/7	15/13/10/6	15/13/10/5	16/14/10/-	16/14/11/-
			30A	16/14/11/7	16/14/10/6	16/14/10/6	16/14/11/-	16/14/11/-



Site I - ACM 20 Verification



Unclassified




- Tested a lab based unit in the field
- ACM20 was designed for online but outside the scope of this evaluation
- Compared the data between the ACM20 and the IOS (upstream)



Site I - ACM 20 Verification



Unclassified

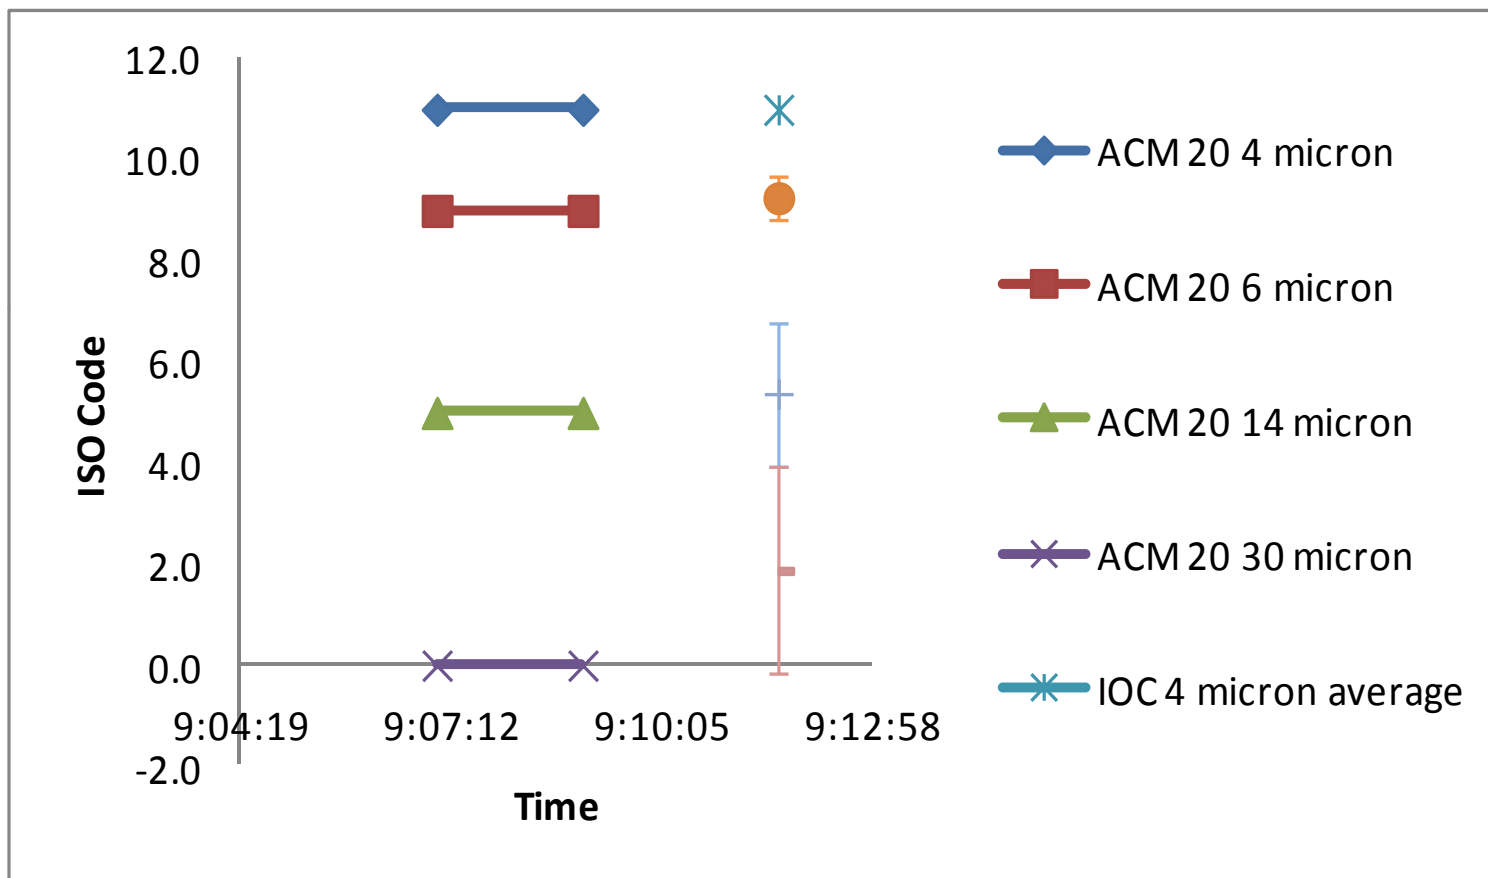



Site I - ACM 20 Verification




Unclassified

Time (EST)	Location	Lab ID	Avcount	ACM20 On-line	ACM20 #1	ACM20 #2	S40 AVTUR #1	S40 AVTUR #2
845	Upstream	32	17/15/11/7		15/13/9/5	15/13/9/5	16/14/10/-	16/14/10/-
		32A	17/15/11/7		16/14/10/6	16/14/10/6	16/14/11/-	16/14/11/-
900	Upstream	33	16/14/10/7		16/14/10/0	16/14/10/4	17/14/11/-	17/14/11/-
		33A	17/15/11/8		16/14/10/5	17/14/10/5	17/15/11/-	17/15/11/-
907	Upstream			11/9/5/0				
909	Upstream			11/9/5/0				



Site I - Bulk Sampling ACM 20 Verification


Unclassified

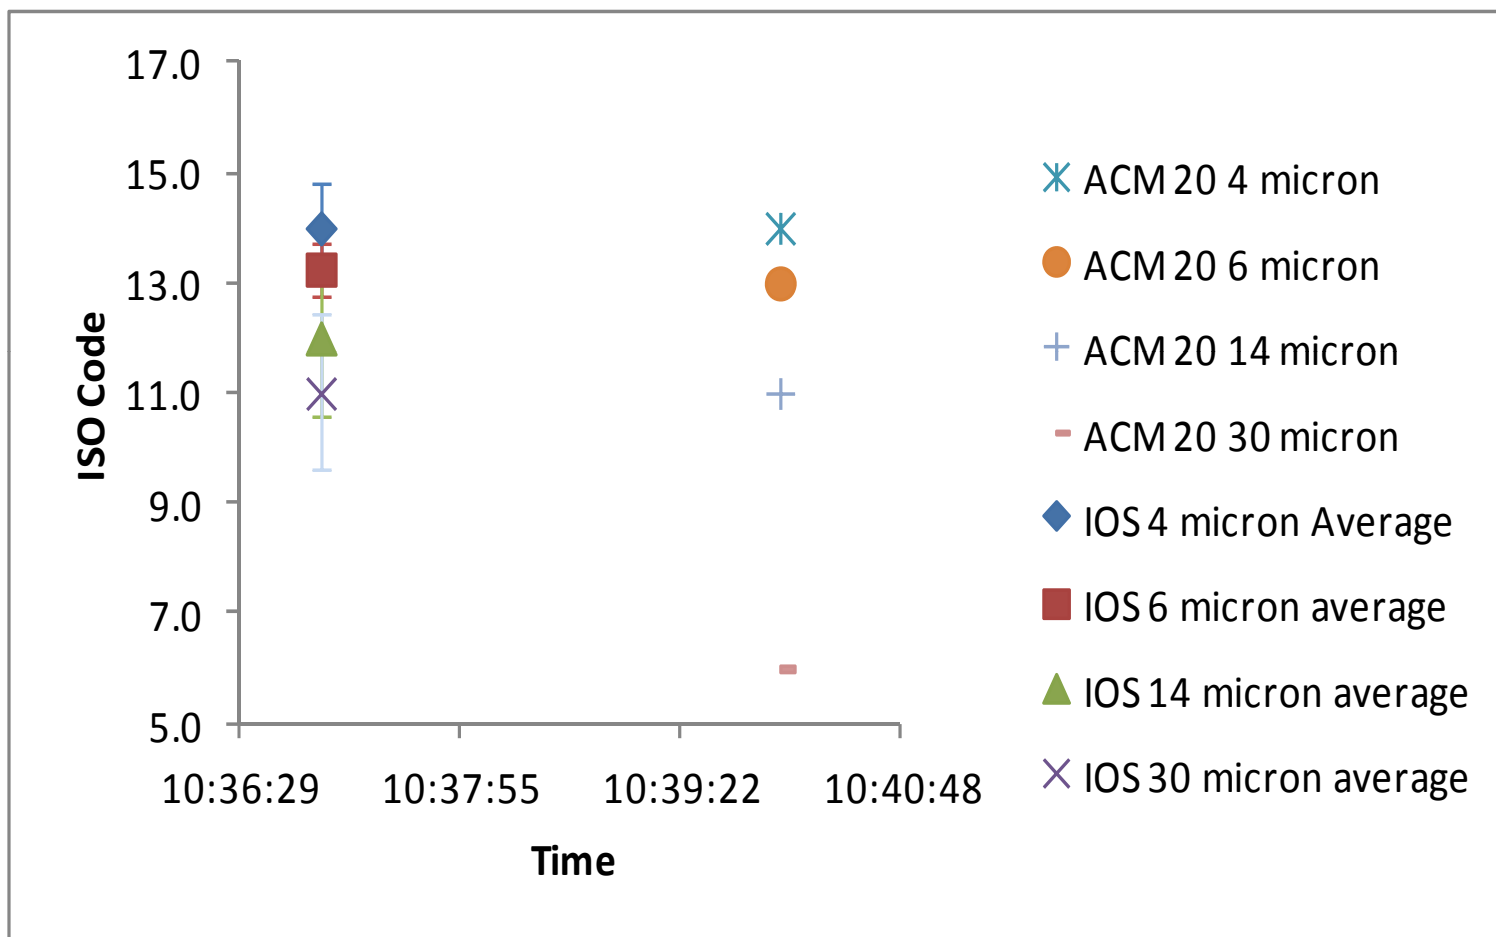



Site I - Bulk Sampling ACM 20 Verification

Unclassified

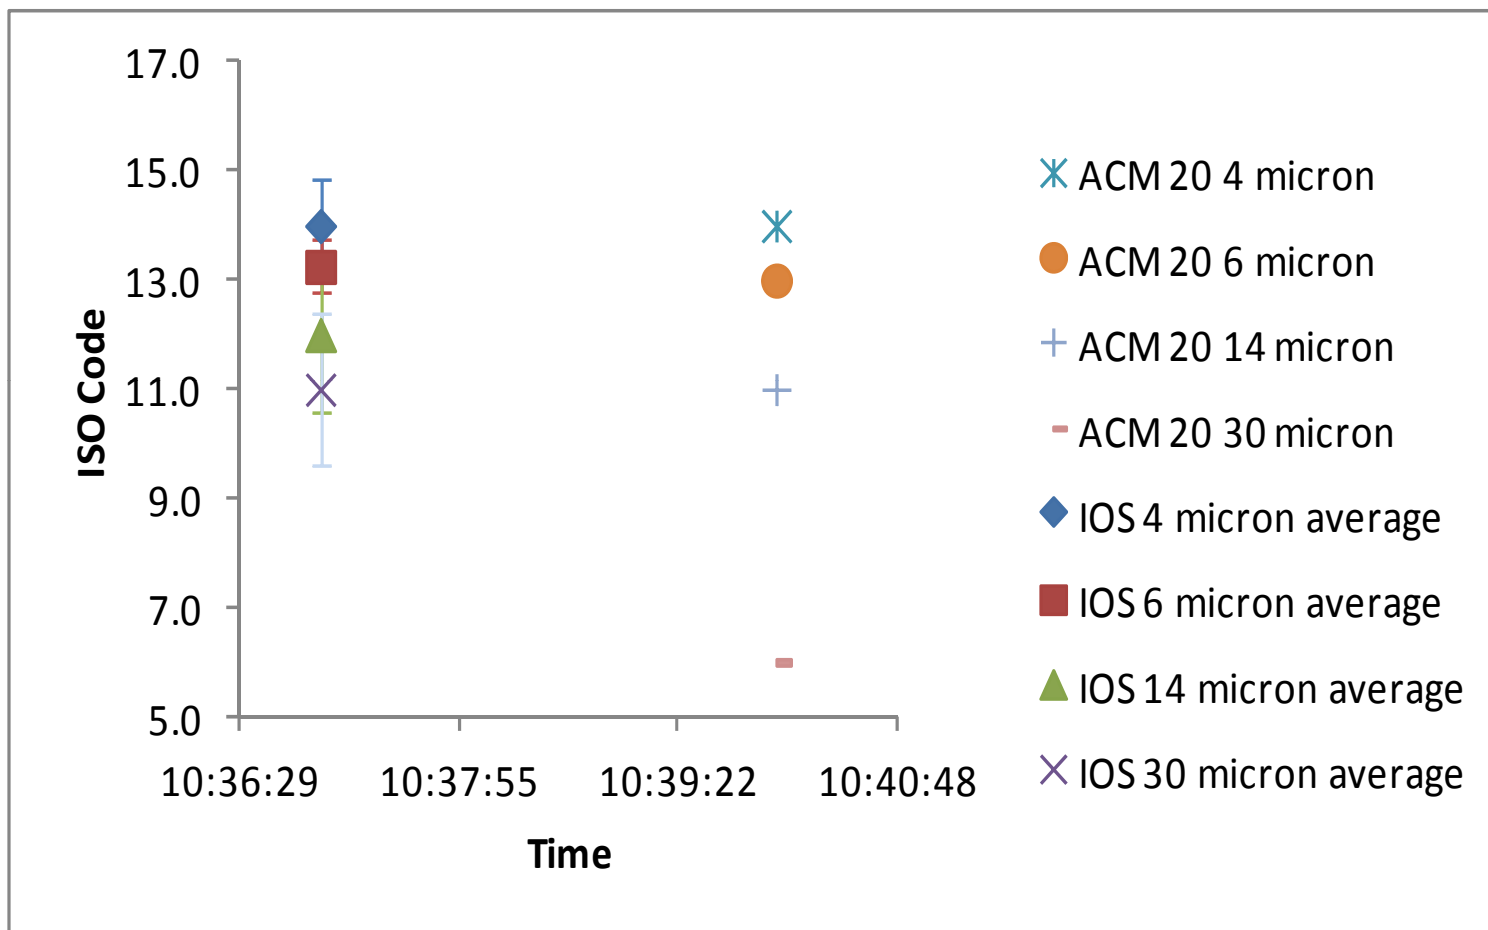



Site I - Bulk Sampling ACM 20 Verification

Unclassified



Time (EST)	Truck	Location	Lab Unit Run ID	Avcount	ACM-20 On-line	ACM-20 #1	ACM-20 #2	S40 AVTUR #1	S40 AVTUR #2
1014	6	Bulk	35	16/14/11/9	14/13/11/6	16/13/11/10	16/13/10/8	16/14/12/-	16/14/11/-
			35A	17/14/12/11		16/14/12/12	16/14/12/11	16/14/13/-	16/15/13/-
1030	7	Bulk	36	17/14/11/9	12/11/6/6	16/14/10/6	16/14/10/6	16/14/11/-	16/14/11/-
			36A	17/15/11/9		16/14/10/6	16/14/10/6	17/15/11/-	17/14/11/-




U.S. ARMY
RDECOM
RESEARCH DEVELOPMENT ENGINEERING CENTER

Site II – Fuel Distribution Overview



Unclassified

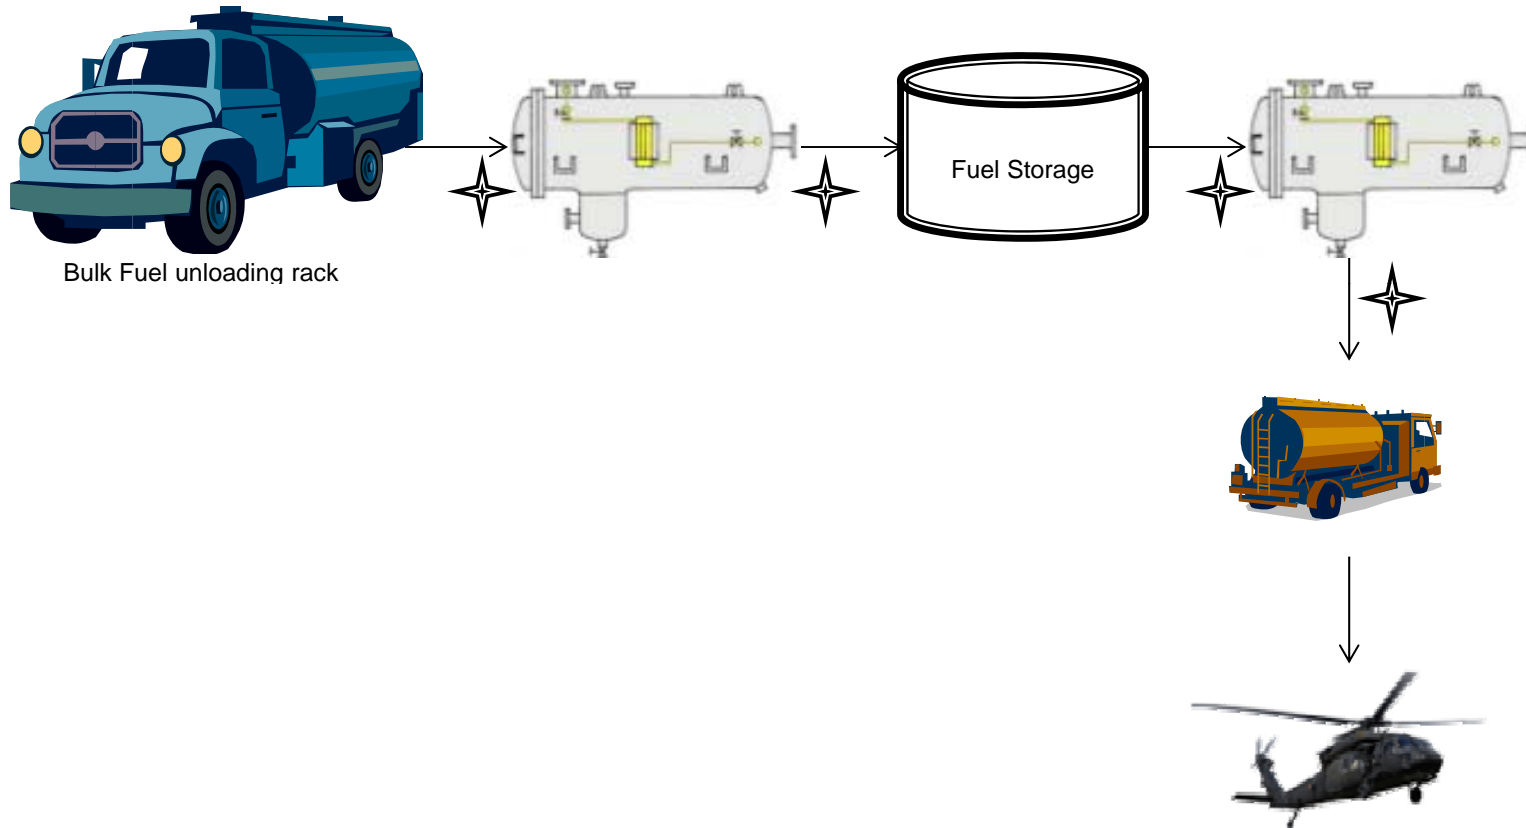



Site II - Samples

Unclassified




Sample #	Date	Time (EST)	Sample Source/Location	Sample #	Date	Time (EST)	Sample Source/Location
1	15-Apr-2013	930	Location A AHP Reciept upstream	19	16-Apr-2013	1300	Location A AHP Reciept upstream
2	15-Apr-2013	930	Location A AHP Reciept downstream	20	16-Apr-2013	1300	Location A AHP Reciept downstream
3	15-Apr-2013	1340	Location A AHP Issue upstream	21	17-Apr-2013	915	Location B AHP air pad 11
4	15-Apr-2013	1300	Location A AHP Issue downstream	22	17-Apr-2013	938	Location B AHP air pad 11
5	15-Apr-2013	1300	Location A AHP Issue upstream	23	17-Apr-2013	1330	Location C AHP Reciept upstream
6	15-Apr-2013	1340	Location A AHP Issue downstream	24	17-Apr-2013	1330	Location C AHP Reciept downstream
7	15-Apr-2013	1400	Location A AHP Reciept upstream	25	17-Apr-2013	1408	Location C AHP issue upstream
8	15-Apr-2013	1400	Location A AHP Reciept downstream	26	18-Apr-2013	840	Location C AHP Reciept upstream
9	15-Apr-2013	1435	Location A AHP Issue upstream	27	18-Apr-2013	840	Location C AHP Reciept downstream
10	15-Apr-2013	1435	Location A AHP Issue downstream	28	18-Apr-2013	930	Location C AHP Reciept upstream
11	15-Apr-2013	1355	Location A AHP Issue upstream	29	18-Apr-2013	930	Location C AHP Reciept downstream
12	15-Apr-2013	1355	Location A AHP Issue downstream	30	18-Apr-2013	1347	Location C AHP Reciept upstream
13	16-Apr-2013	800	Location A AHP Reciept upstream	31	18-Apr-2013	1347	Location C AHP Reciept downstream
14	16-Apr-2013	800	Location A AHP Reciept downstream	32	18-Apr-2013	1320	Location C AHP Issue upstream
15	16-Apr-2013	930	Location A AHP Reciept upstream	33	18-Apr-2013	1320	Location C AHP Issue downstream
16	16-Apr-2013	930	Location A AHP Reciept downstream	34	18-Apr-2013	1320	Location C AHP Issue upstream
17	16-Apr-2013	1300	Location A AHP Issue upstream	35	18-Apr-2013	1320	Location C AHP Issue downstream
18	16-Apr-2013	1300	Location A AHP Issue downstream				



Site II - Receipts Upstream



Unclassified

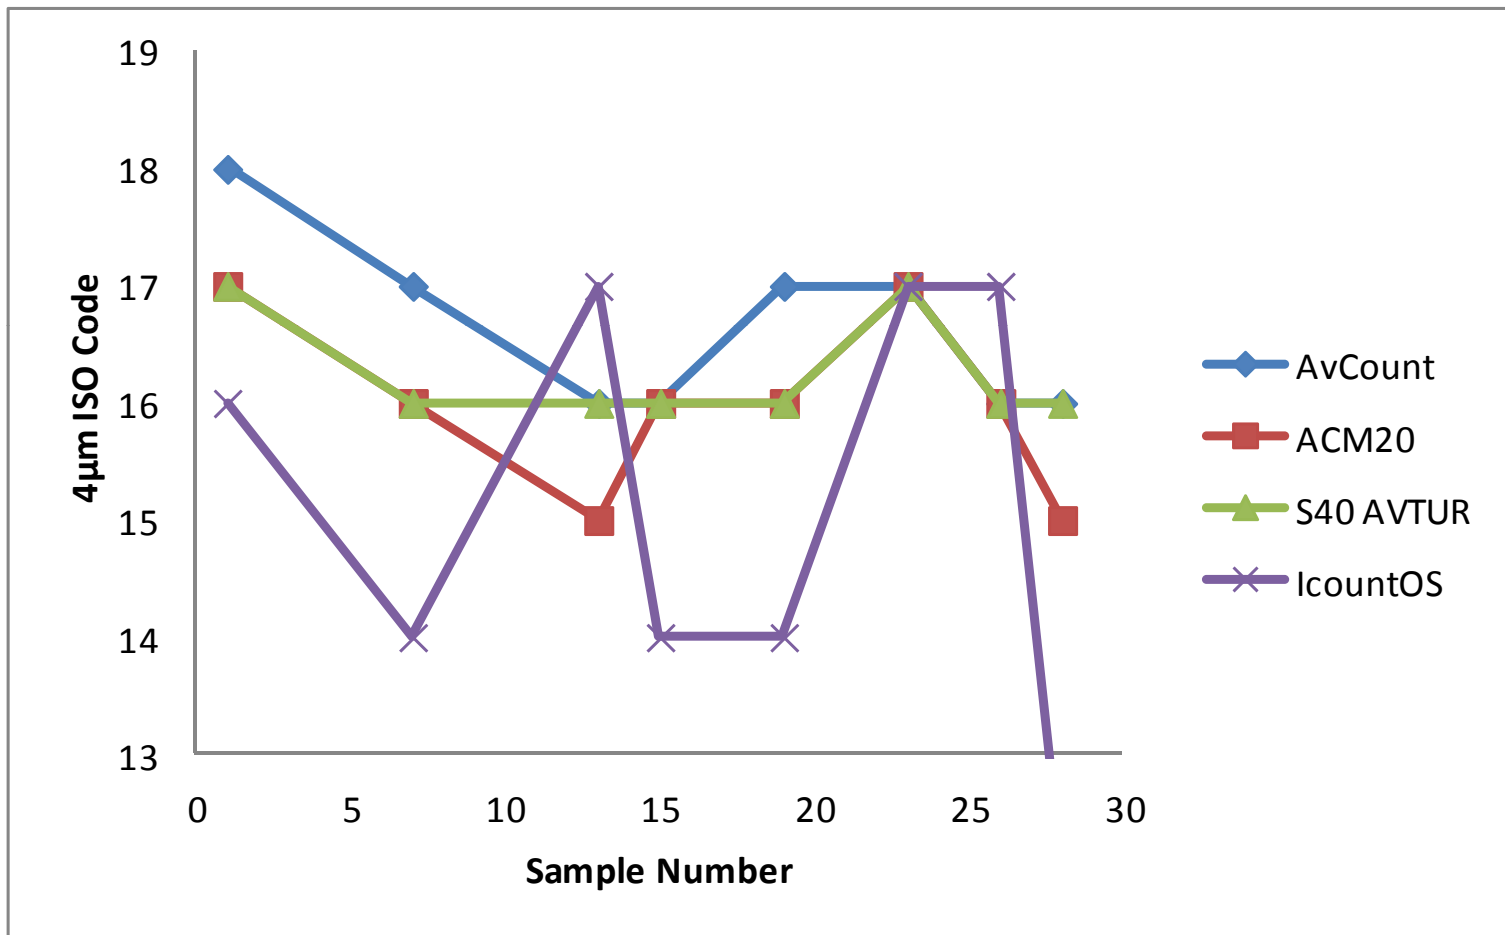




Site II - Receipts Downstream



Unclassified

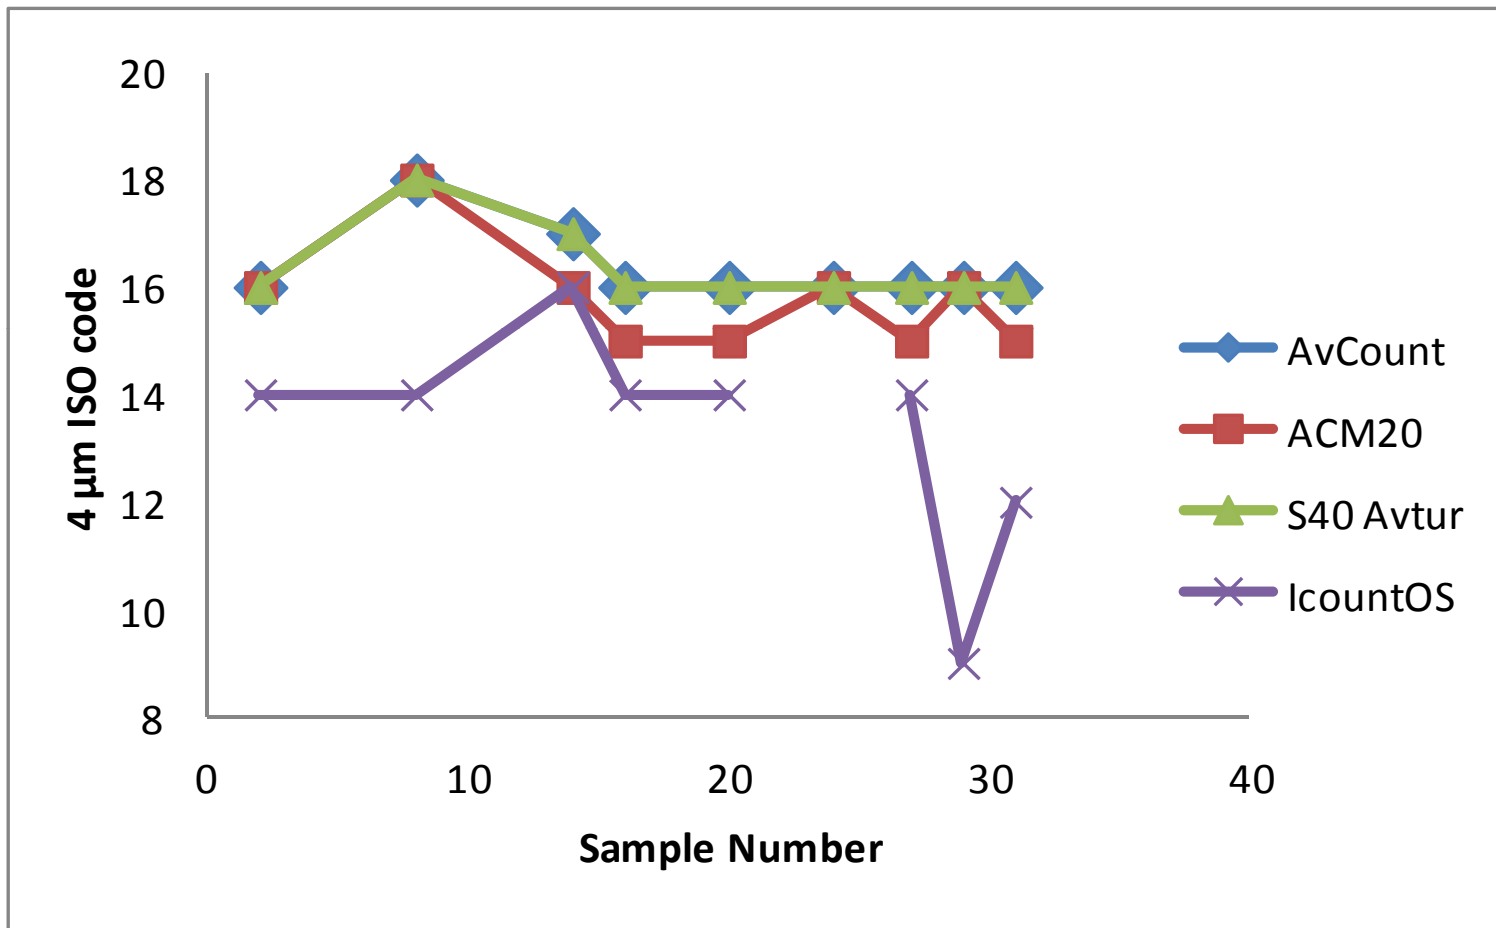




Site II - Receipts Upstream



Unclassified

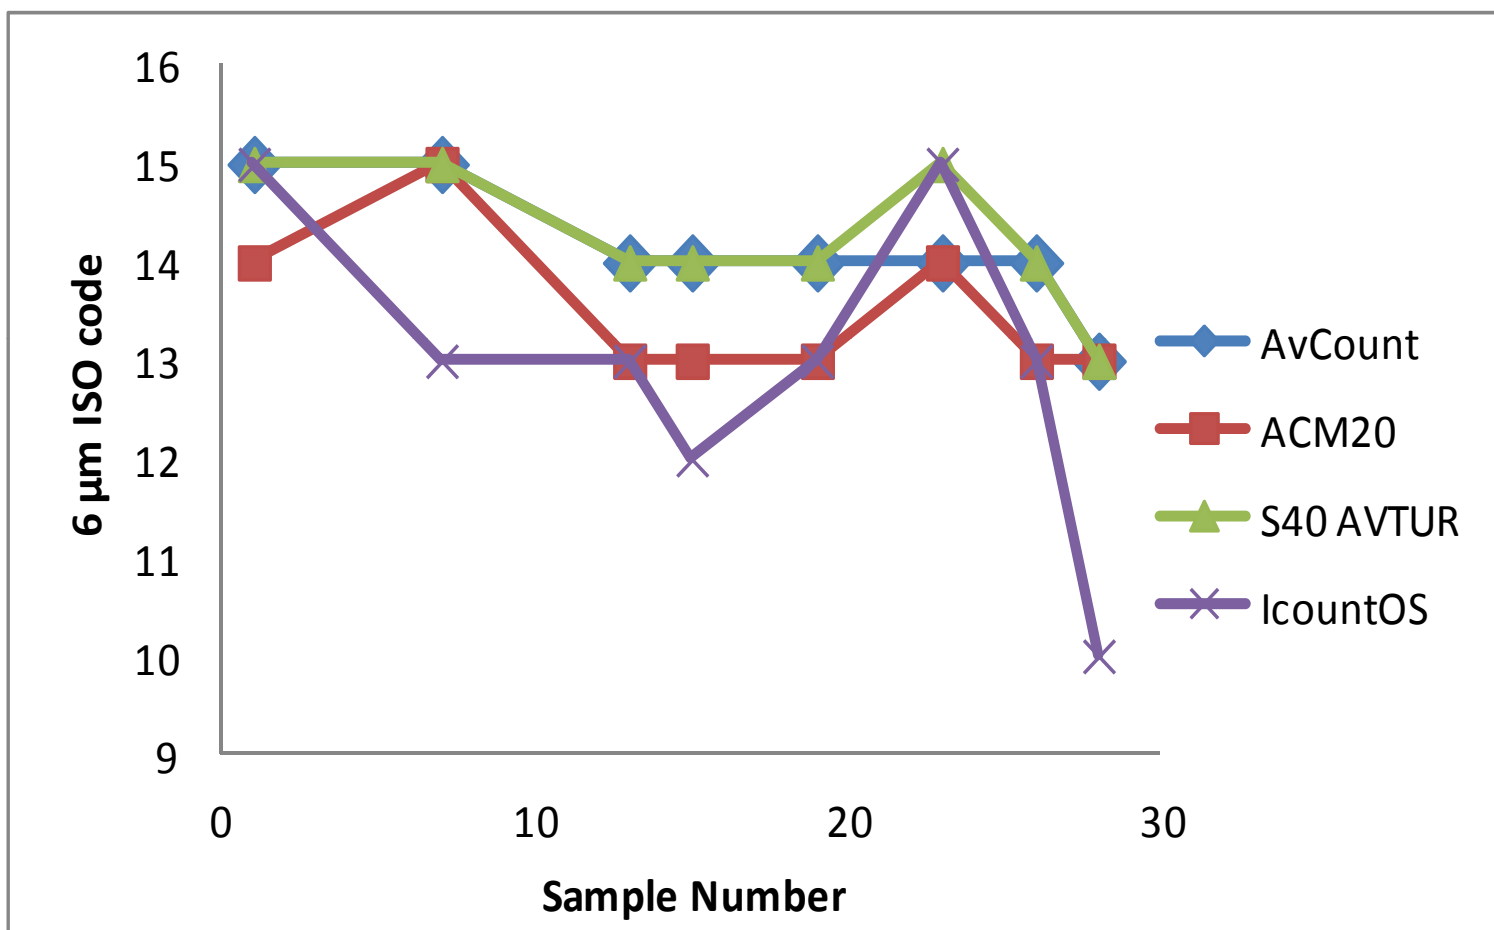




Site II - Receipts Downstream



Unclassified

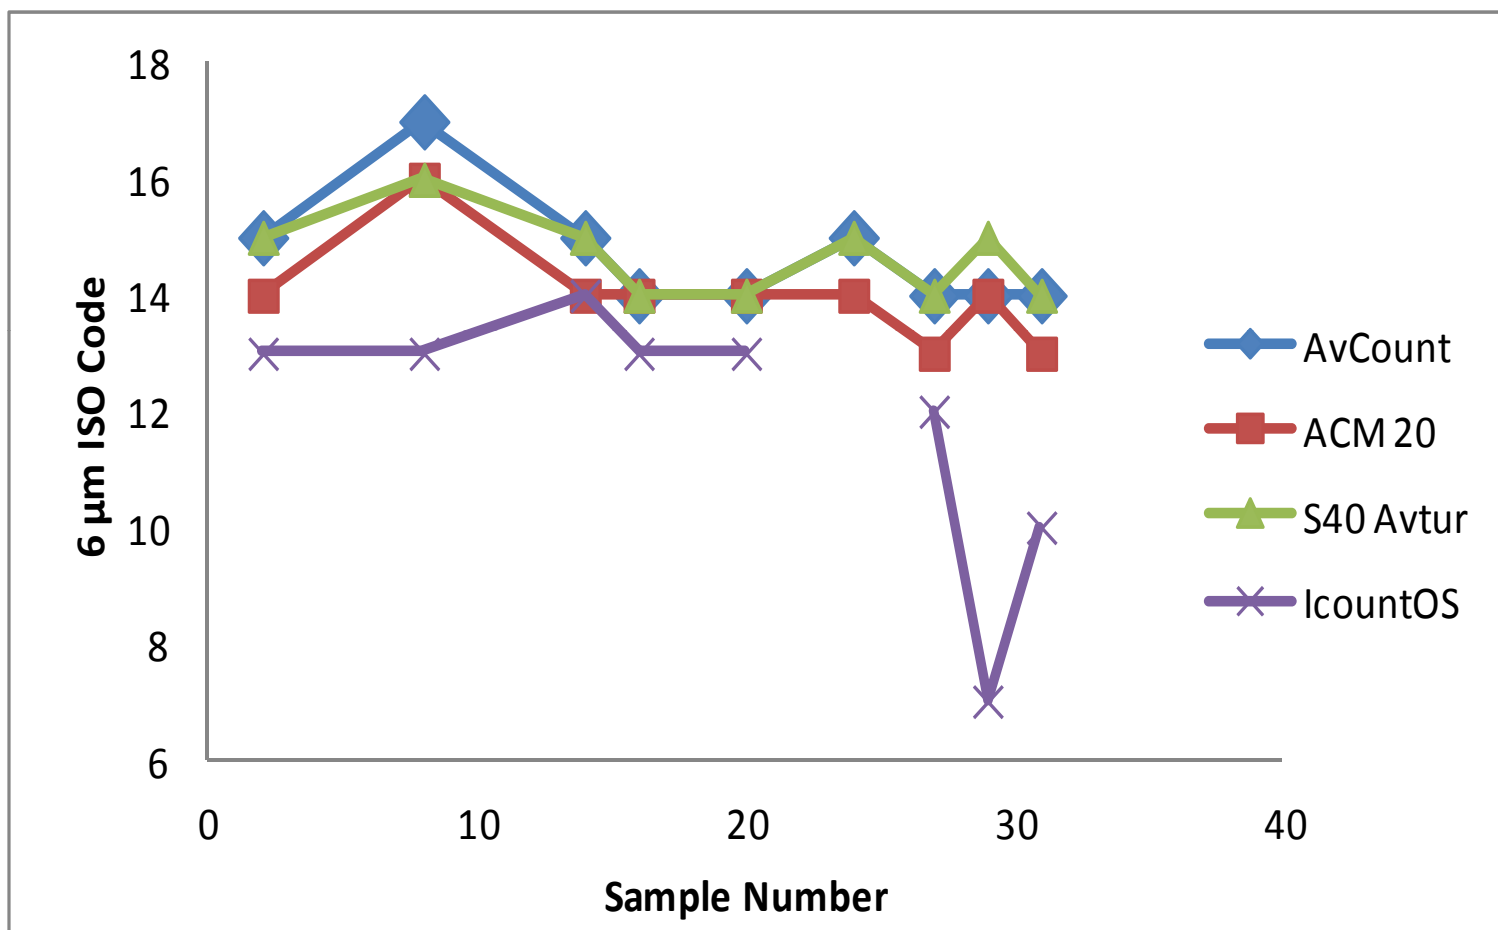



Site II - Receipts

Unclassified



Time (EST)	Location	Sample #	mg/L	Avcount	ACM20	S40 AVTUR	lcountOS
930	upstream	1	0.3	18/15/11/8	17/14/10/6	17/15/11/-	16/15/14/13
930	downstream	2	0.2	16/15/12/9	16/14/11/7	16/15/12/-	14/13/11/7
1400	upstream	7	0.0	17/15/12/10	16/15/12/8	16/15/12/-	14/13/10/9
1400	downstream	8	1.0	18/17/14/10	18/16/13/8	18/16/13/-	14/13/9/6
800	upstream	13	0.8	16/14/10/6	15/13/9/4	16/14/10/-	17/13/9/6
800	downstream	14	0.5	17/15/11/8	16/14/10/6	17/15/11/-	16/14/10/7
930	upstream	15	0.0	16/14/10/7	16/13/10/5	16/14/10/-	14/12/9/6
930	downstream	16	0.0	16/14/11/7	15/14/10/5	16/14/11/-	14/13/9/7
1300	upstream	19	1.0	17/14/11/8	16/13/10/5	16/14/11/-	14/13/11/10
1300	downstream	20	1.7	16/14/11/7	15/14/10/5	16/14/11/-	14/13/10/8
1330	upstream	23	0.7	17/14/11/7	17/14/11/7	17/15/12/-	17/15/13/10
1330	downstream	24	0.4	16/15/11/7	16/14/10/5	16/15/11/-	-
840	upstream	26	1.0	16/14/10/6	16/13/9/4	16/14/10/-	17/13/10/6
840	downstream	27	0.4	16/14/11/7	15/13/10/7	16/14/10/-	14/12/9/7
930	upstream	28	0.1	16/13/9/6	15/13/8/4	16/13/9/-	12/10/6/0
930	downstream	29	0.1	16/14/10/6	16/14/11/9	16/15/11/-	9/7/0/0



Site II – Location A



Unclassified

Filter Separator Systems

Refueling

Issuing FS; 1 for each stand



Bulk Delivery

Receipt FS; 1 for each stand





Site II – Location A

Unclassified




- Samples taken upstream and downstream of the Filter Separator
 - ✓ IOS (online)
 - ✓ Matched weight monitor
 - ✓ Aqua-Glo
- Refueling trucks were small (~2500gals) and would fill before we could pull gravimetrics and Aqua-Glo samples



Site II – Location A – Samples 1 & 2



Unclassified

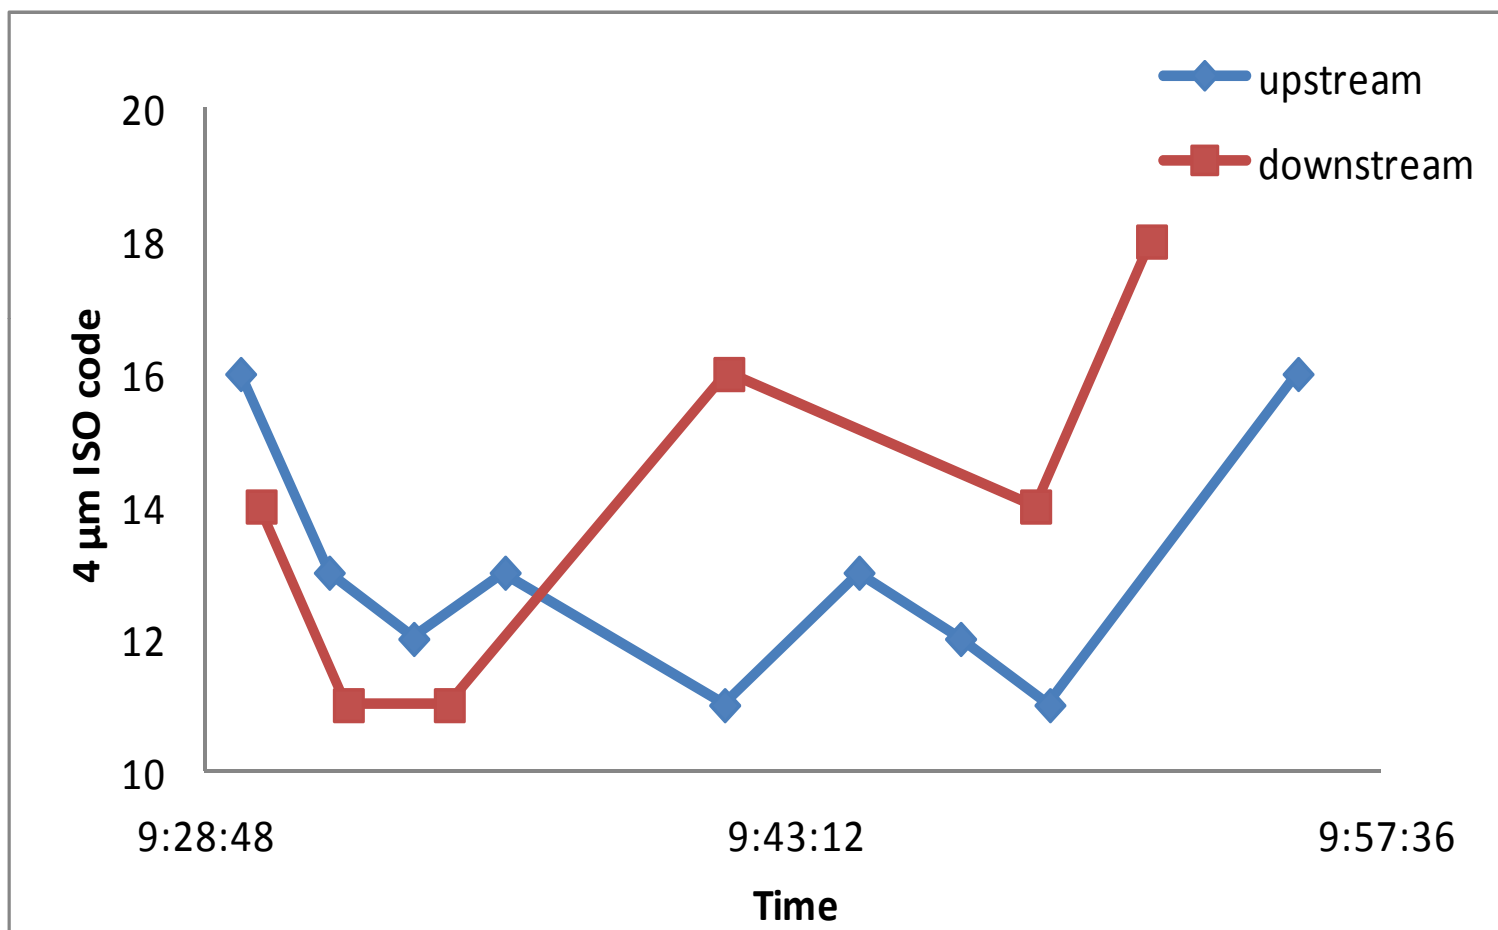




Site II – Location A – Samples 7 & 8



Unclassified

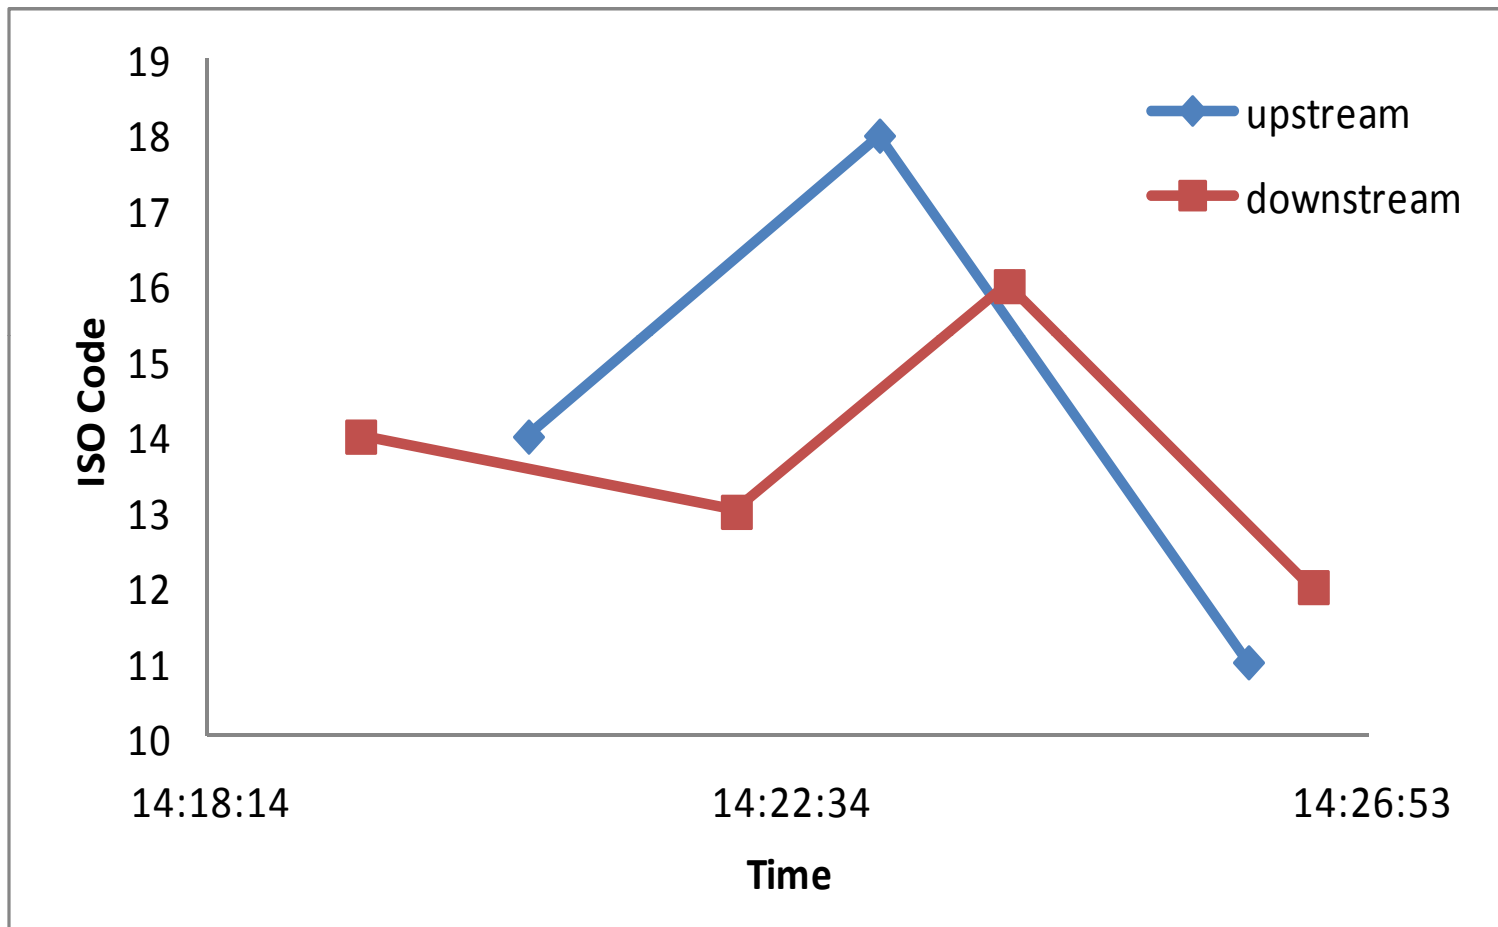




Site II – Location A – Samples 13 & 14



Unclassified

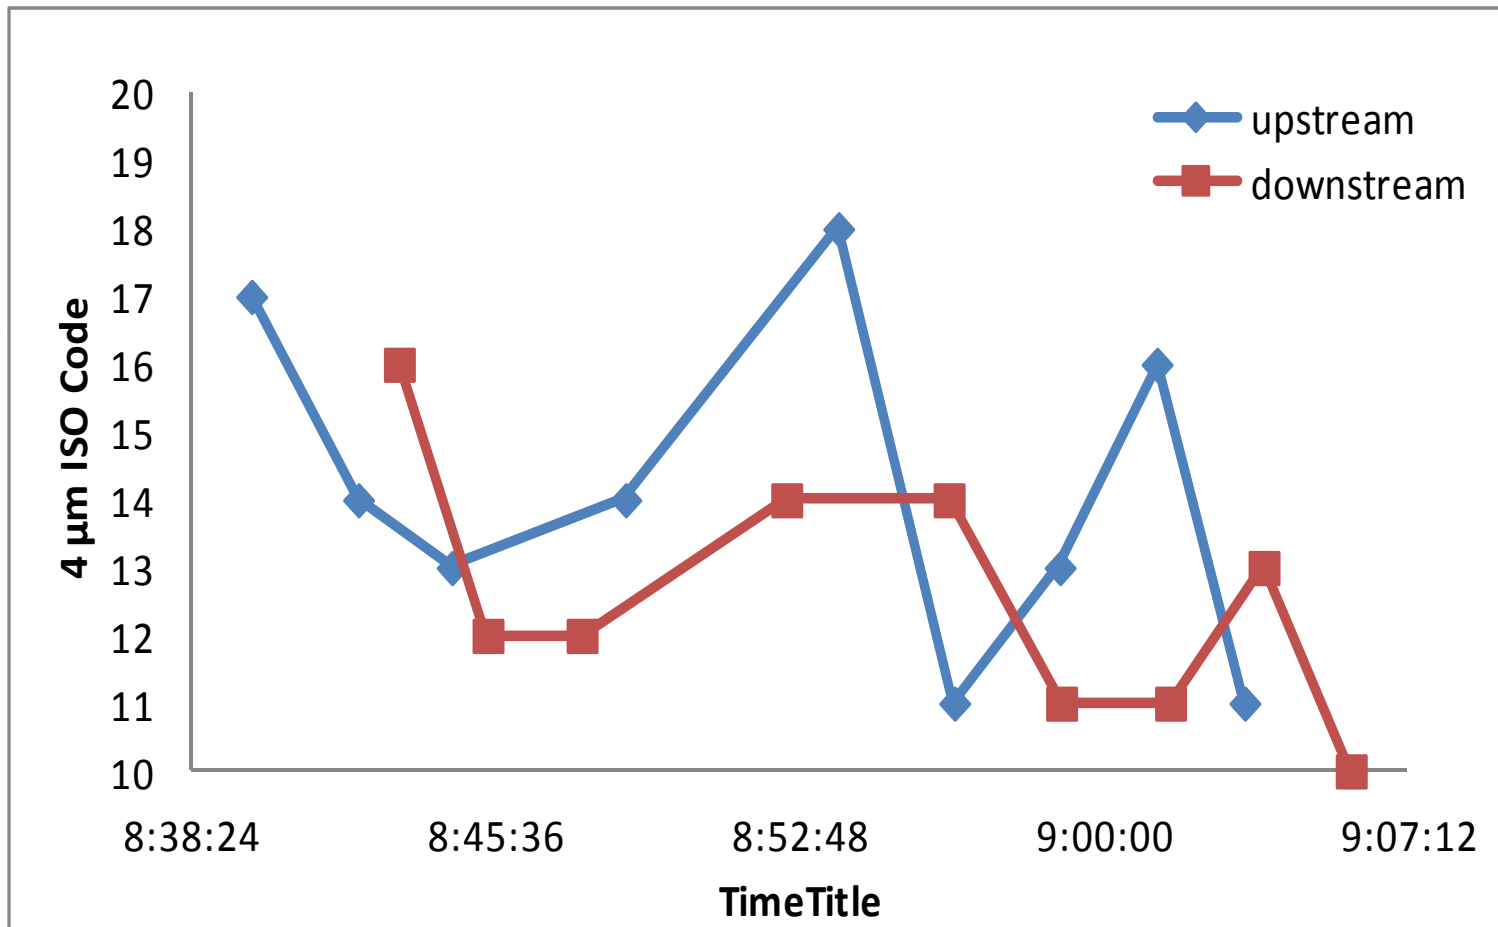




Site II – Location A – Sample 15



Unclassified

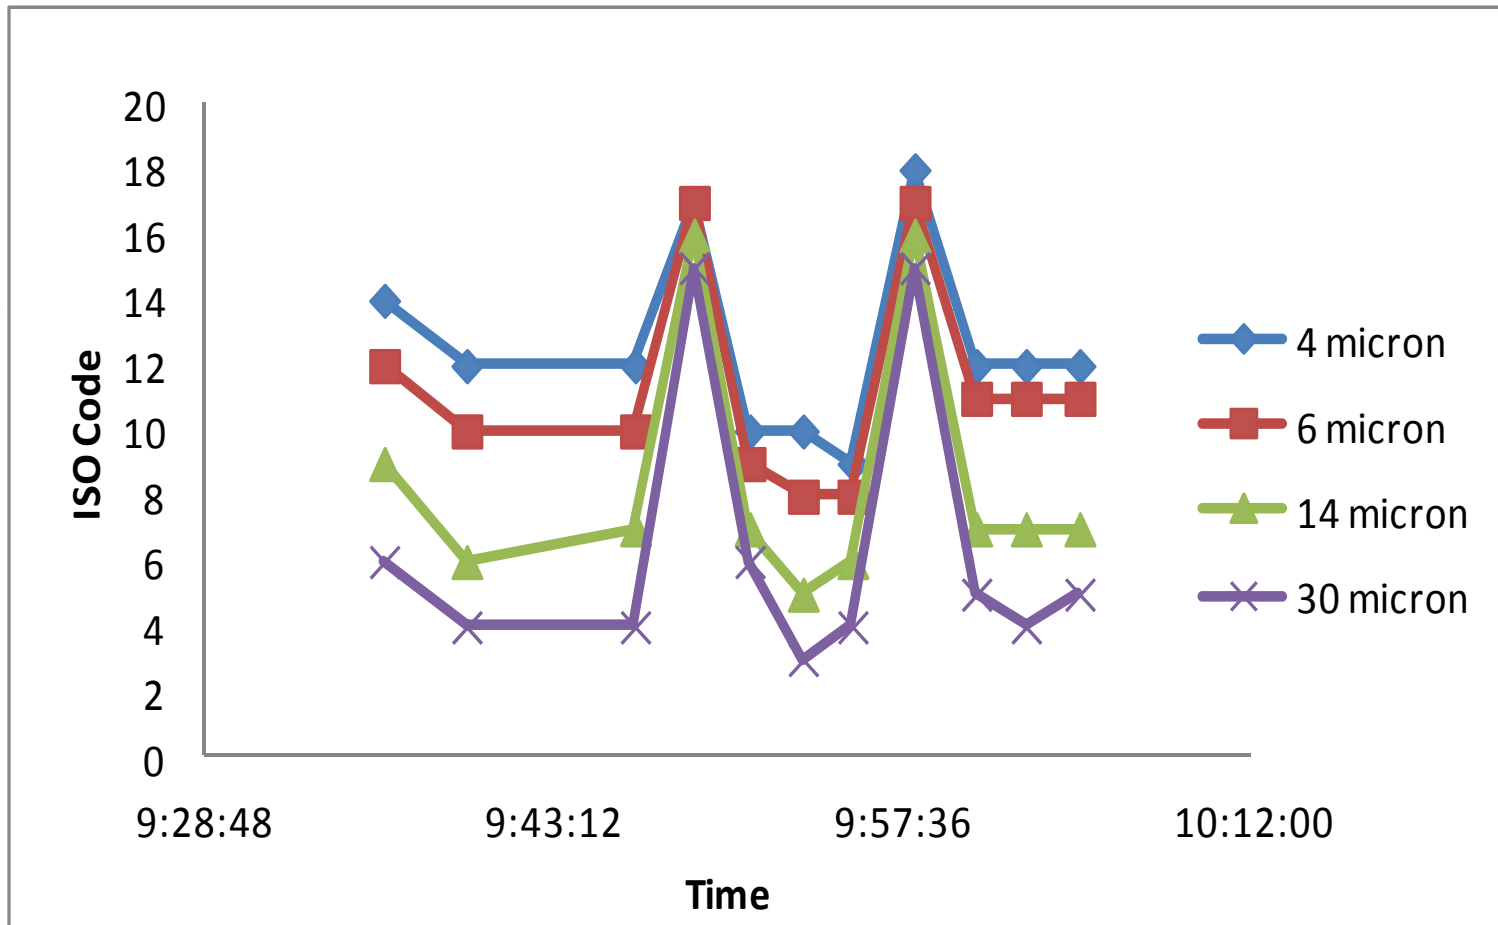




Site II – Location A – Sample 16



Unclassified

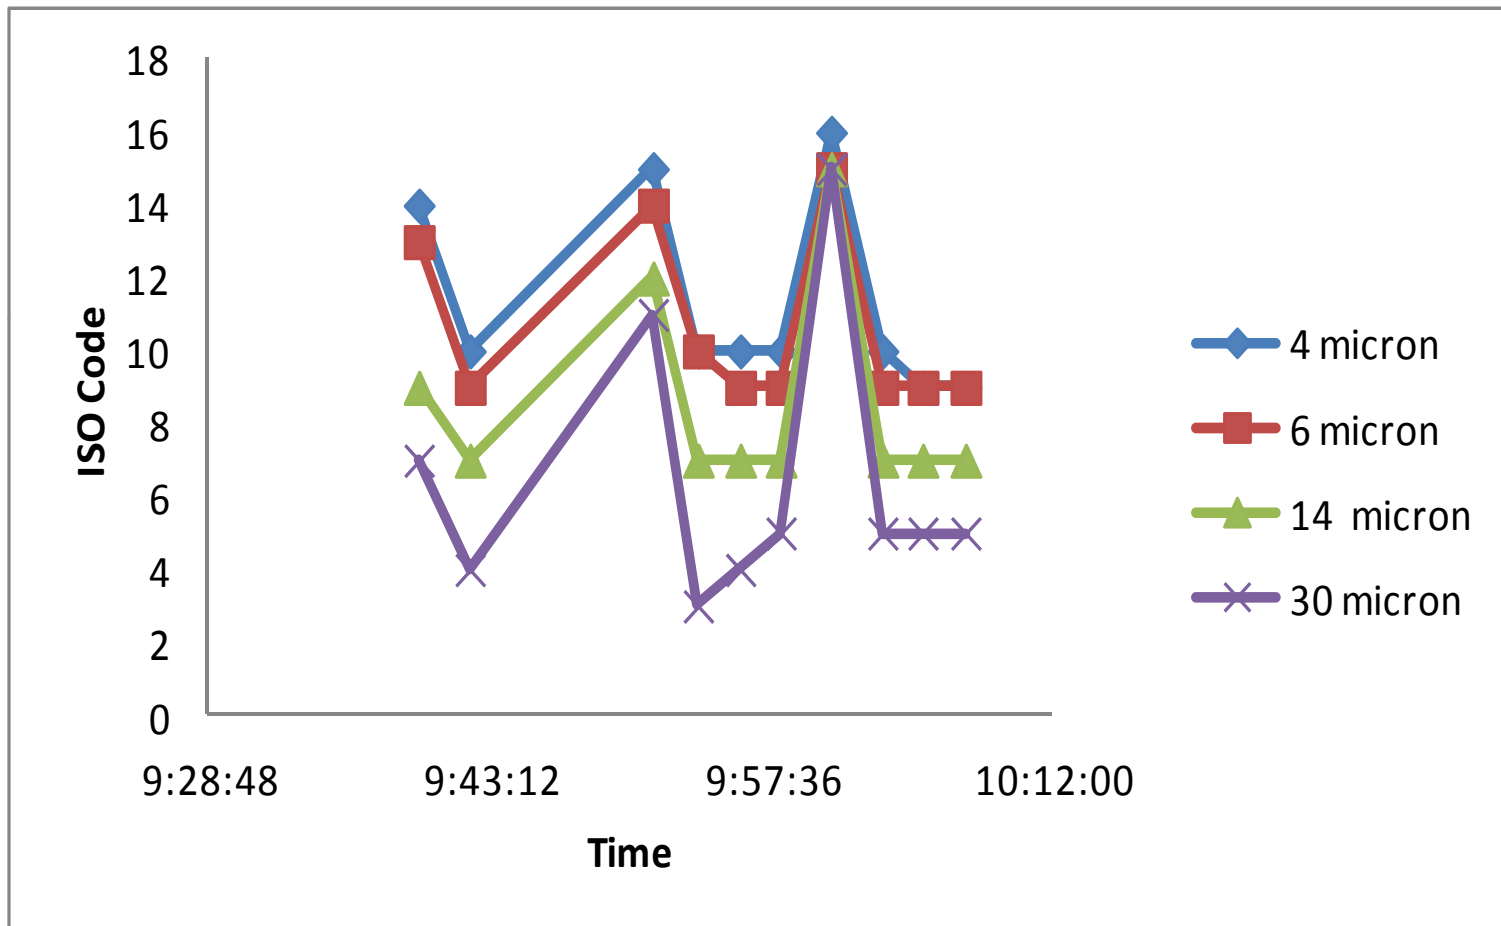




Site II – Location A – Samples 19 & 20



Unclassified

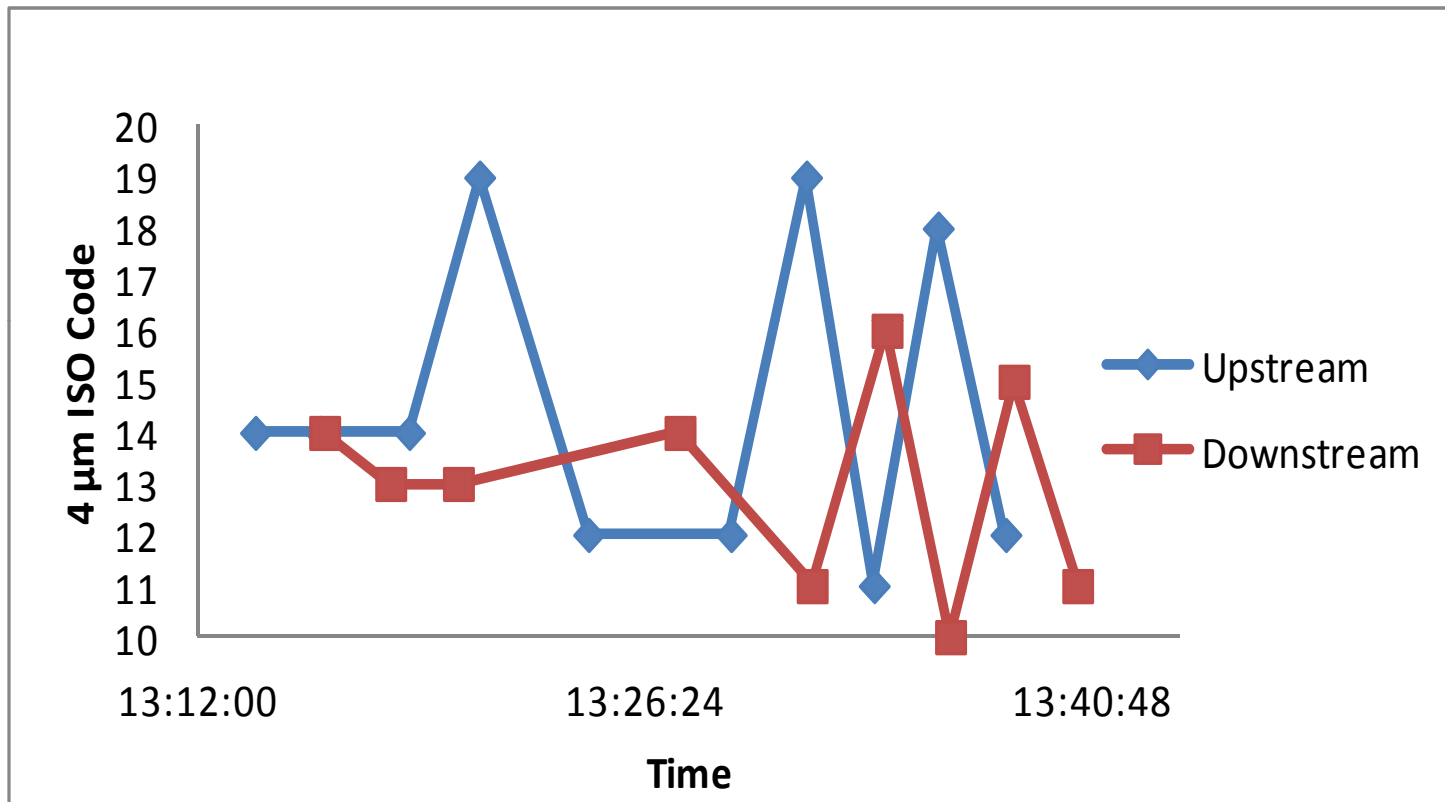




Site II – Location A – Sample 19



Unclassified

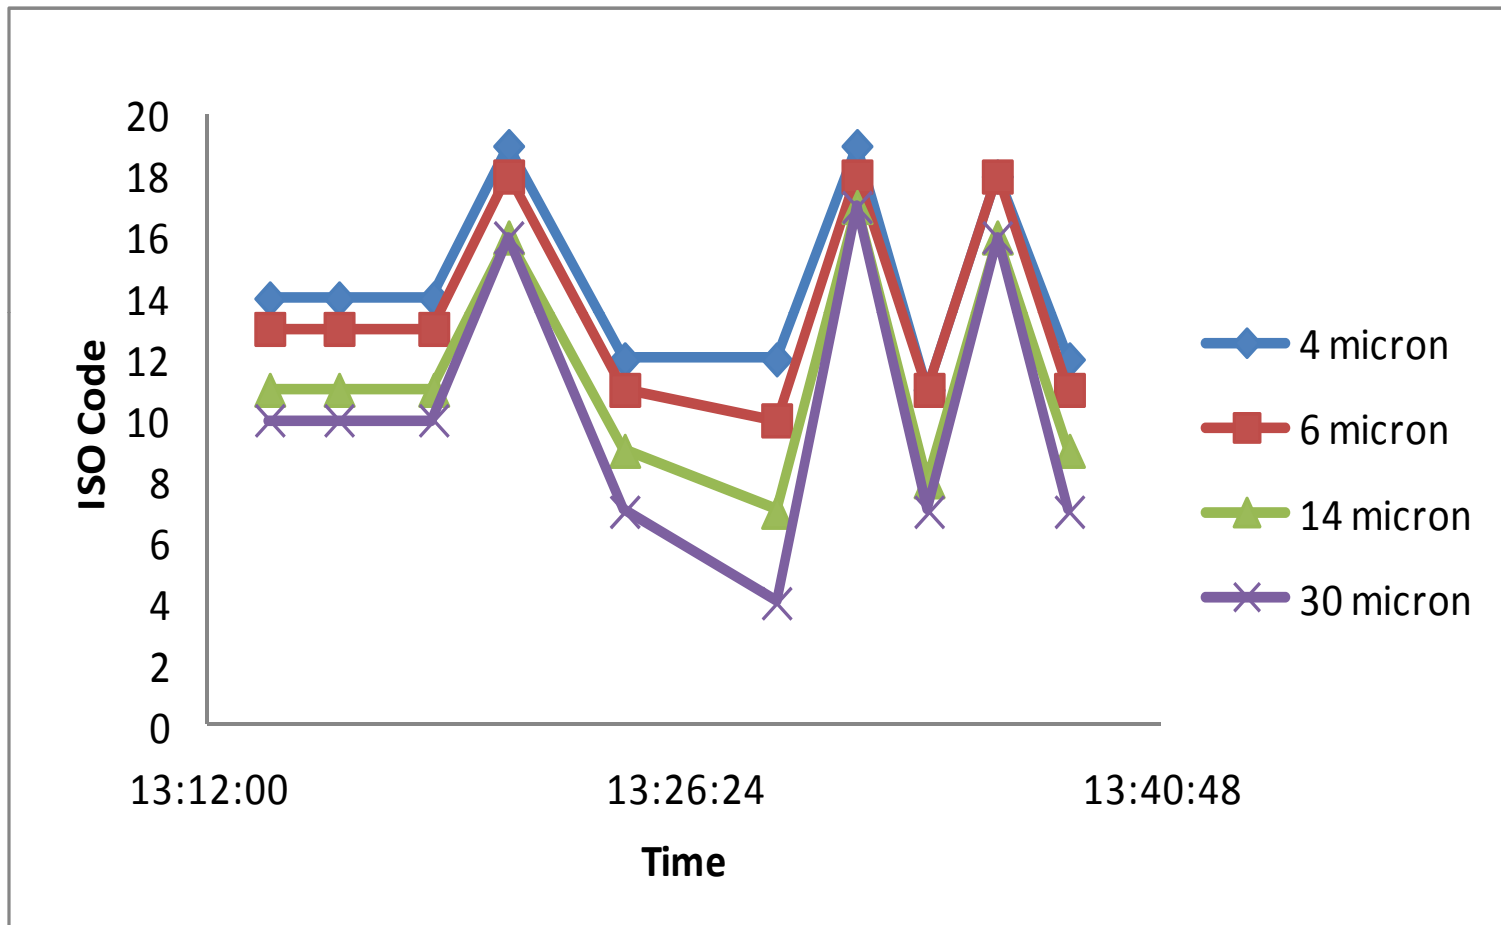




Site II – Location A – Sample 20



Unclassified

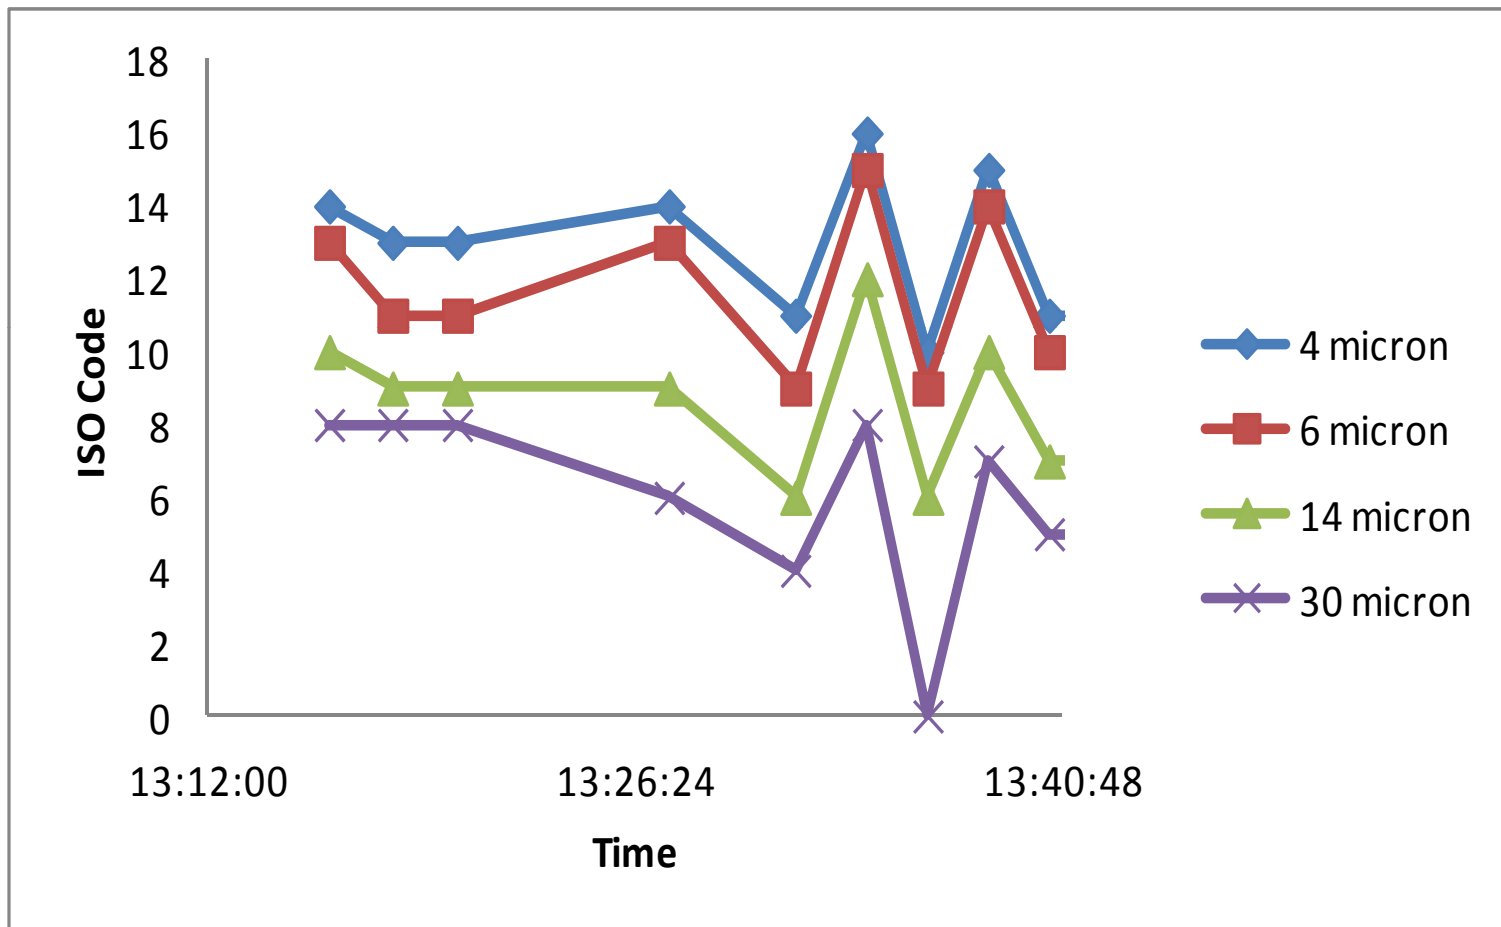



In-line testing Observation



Unclassified


IOS counts would spike during bulk offload. These trucks were baffled and air was introduced to the system when the operators switched tank compartments.





Site II – Location A – Issue 2,4,5,6,11 & 12

Unclassified

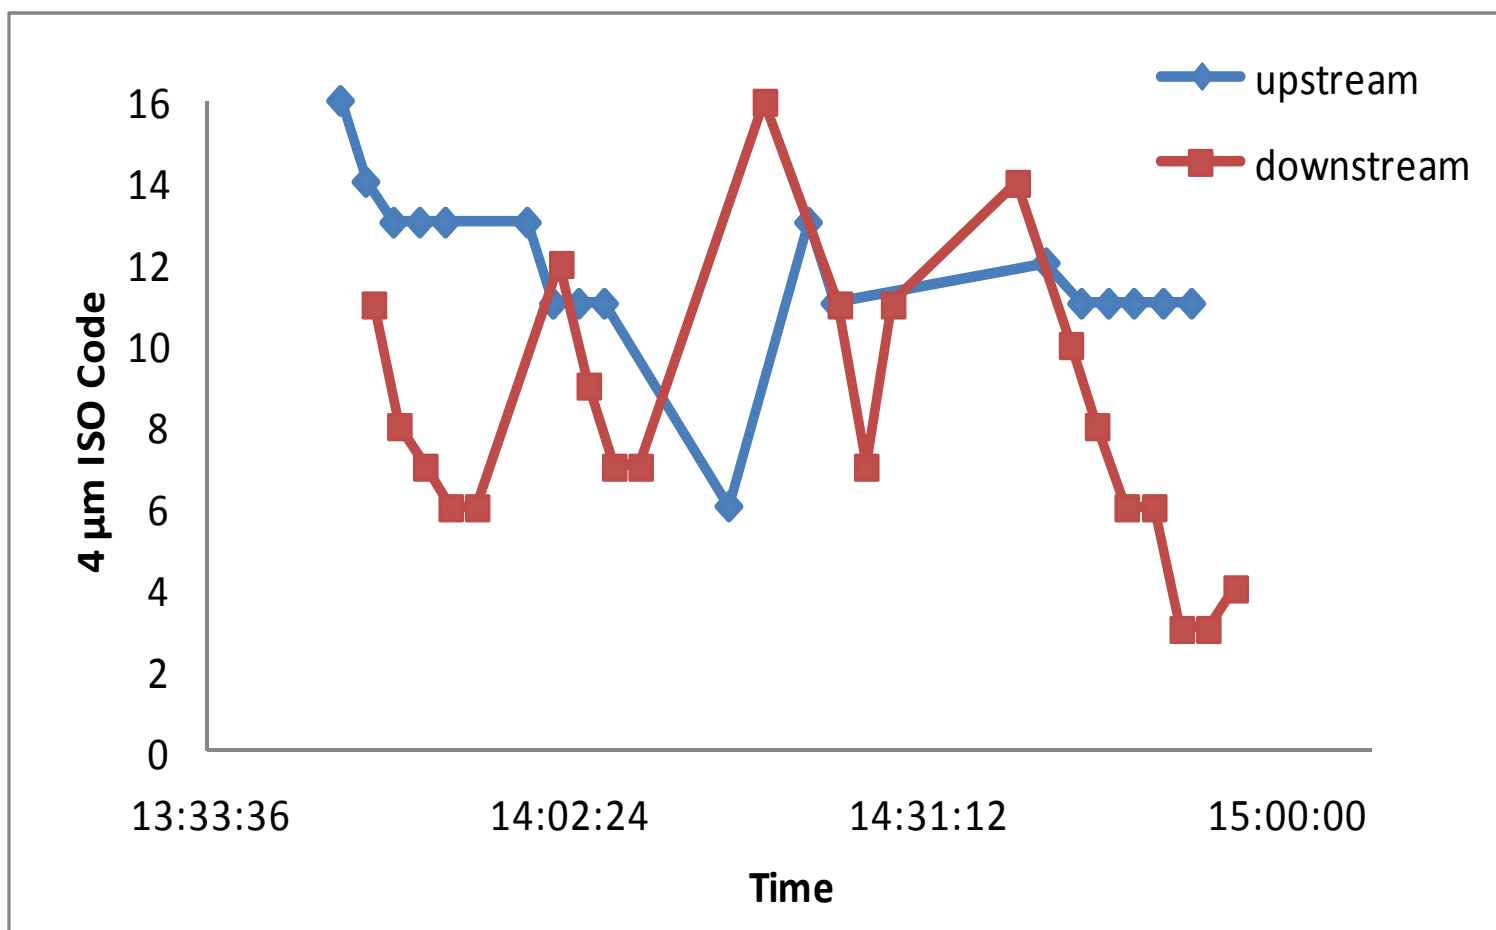




Site II – Location A – Issue 17 & 18



Unclassified

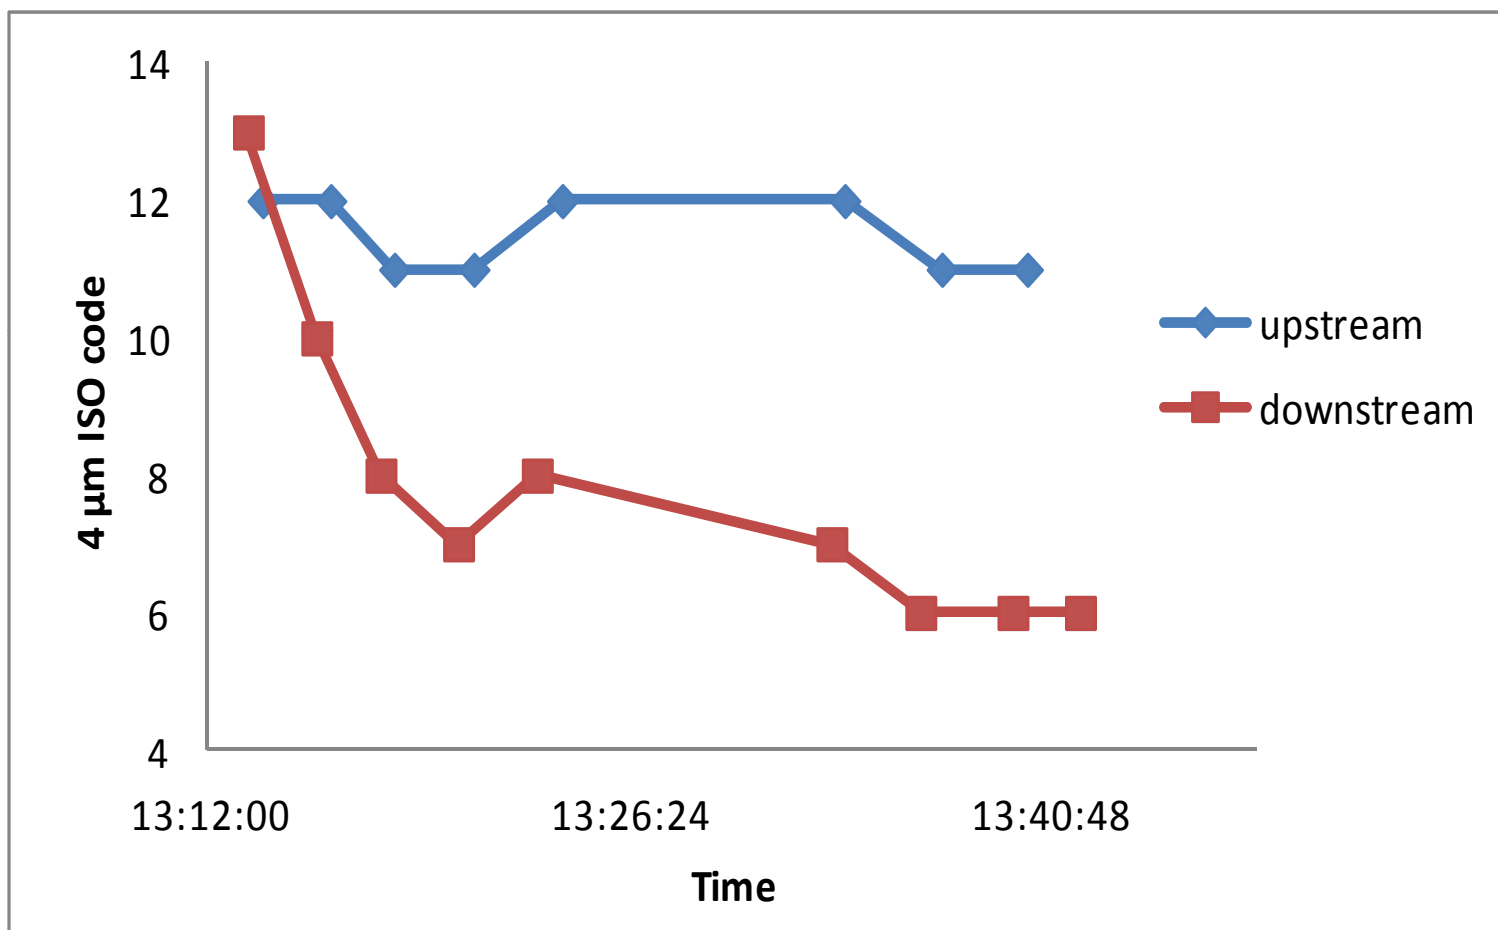



U.S. ARMY
RDECOM
RESEARCH DEVELOPMENT ENGINEERING CENTER

Site II – Location B - Army Heliport



Unclassified

- Hot refueling location
- 2 bulk tanks; 2 receiving FS
- Fuel that isn't issued is refiltered through system
- Typical refuel takes 2-4 minutes






Site II – Location B - Air Pad 11



Unclassified

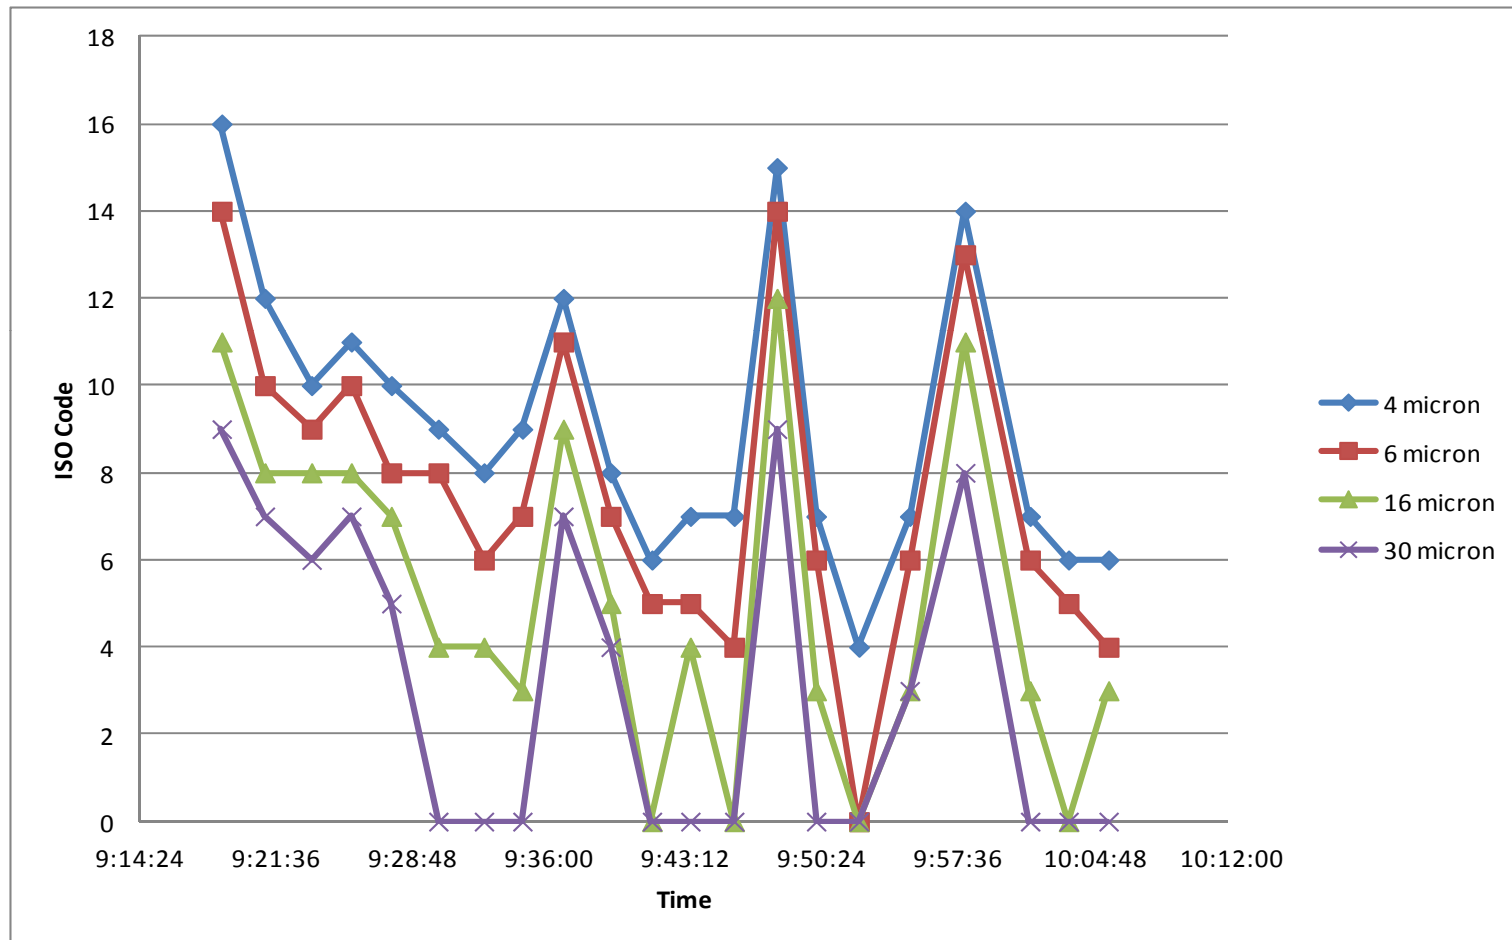



Site II – Location B - Air Pad 11



Unclassified

Time (EST)	Sample #	Avcount	ACM20	S40 AVTUR
915	21	16/14/11/7	16/14/10/6	17/14/11/-
938	22	16/14/10/7	15/13/9/6	16/13/10/-



Site II – Location C Bulk Delivery and Refueling Station



Unclassified






Site II – Location C - Testing



Unclassified

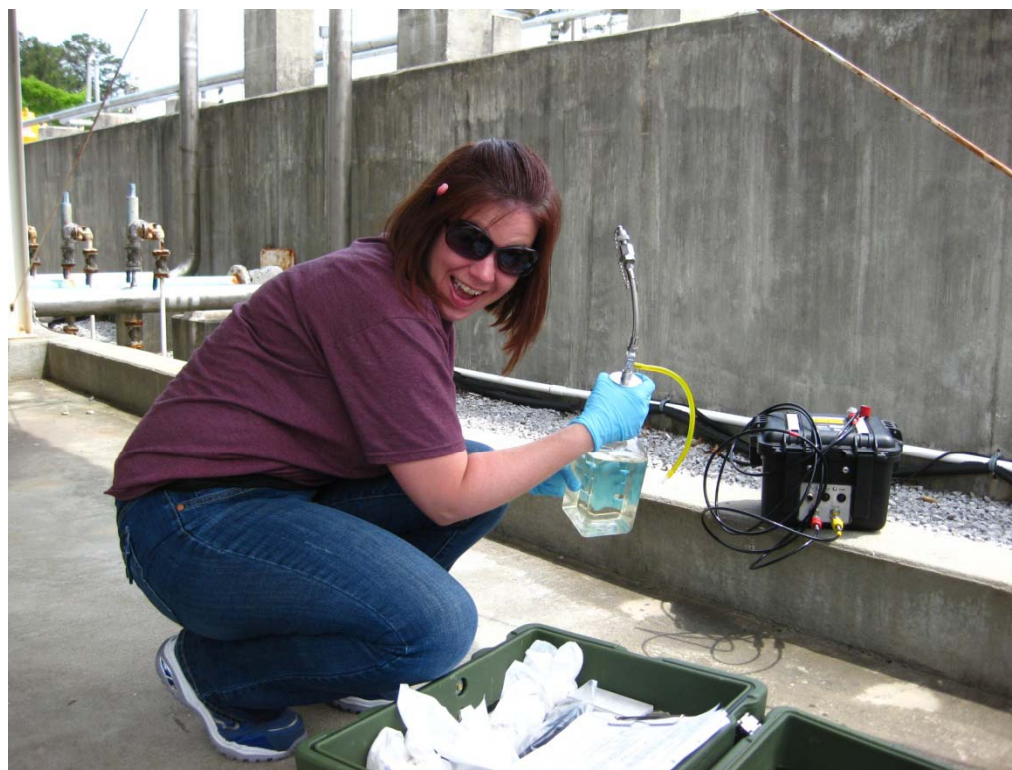



Site II – Location C - Testing



Unclassified



Online IOS testing






Site II – Location C – Samples 26 & 27



Unclassified

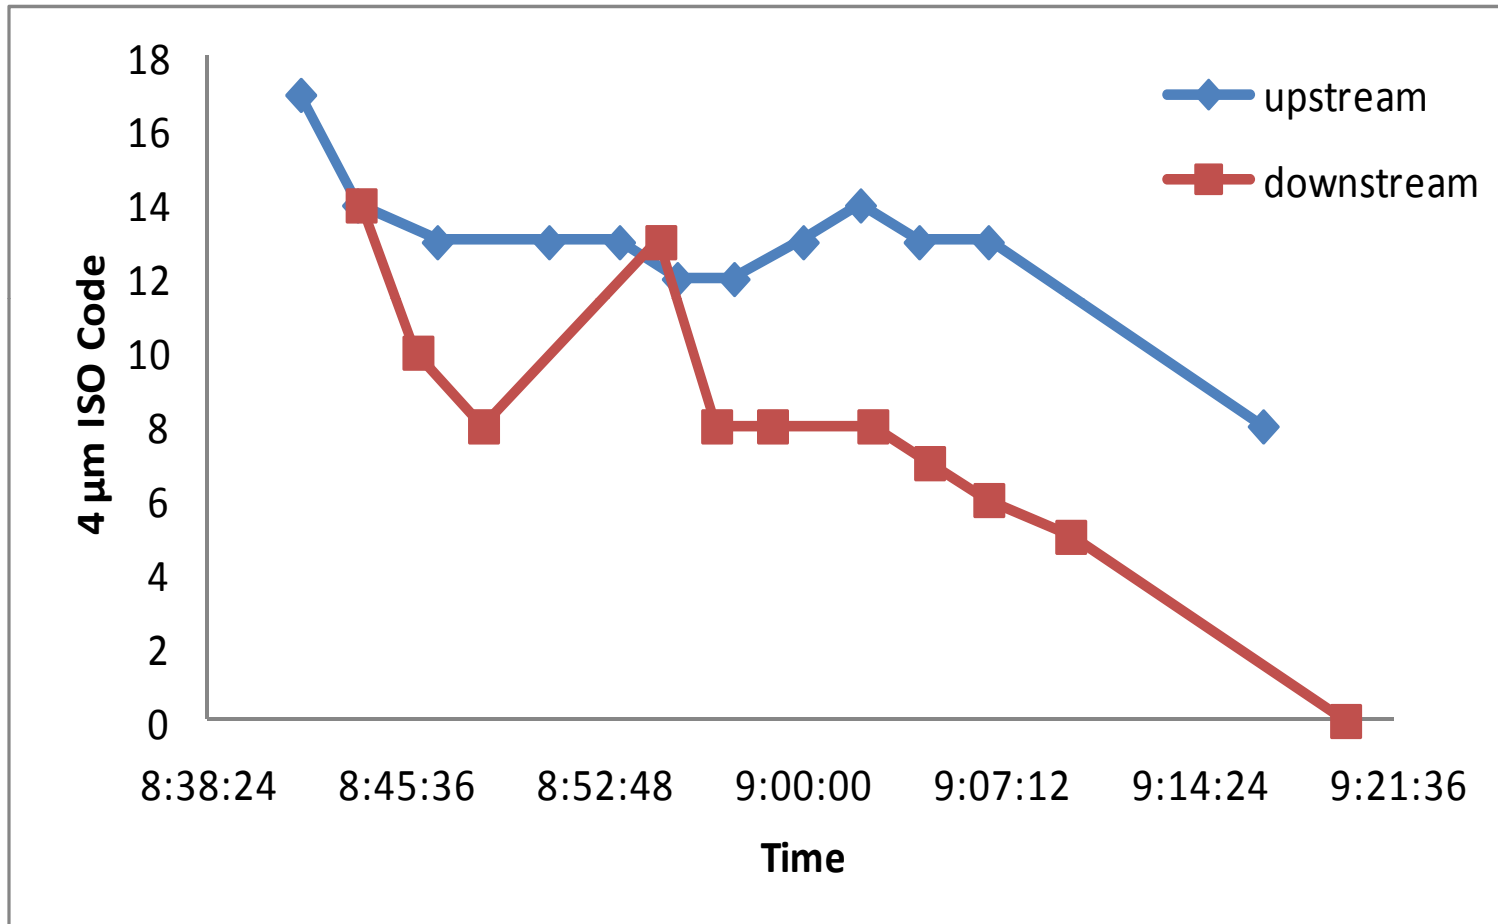




Site II – Location C – Samples 28 & 29




Unclassified

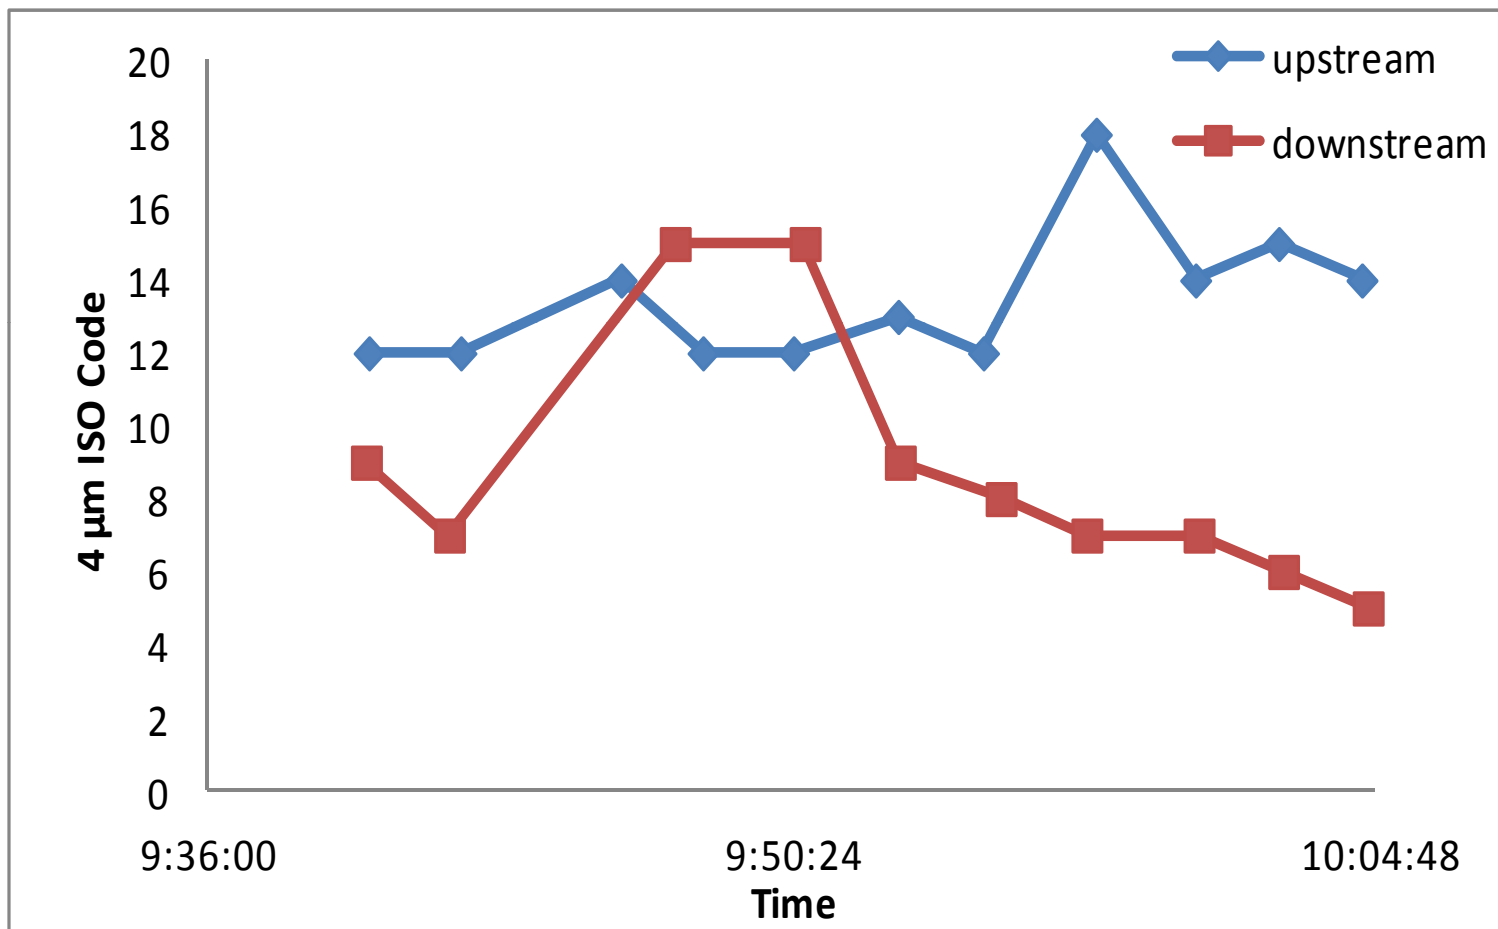



Site II – Location C Issue samples 32 & 33

Unclassified

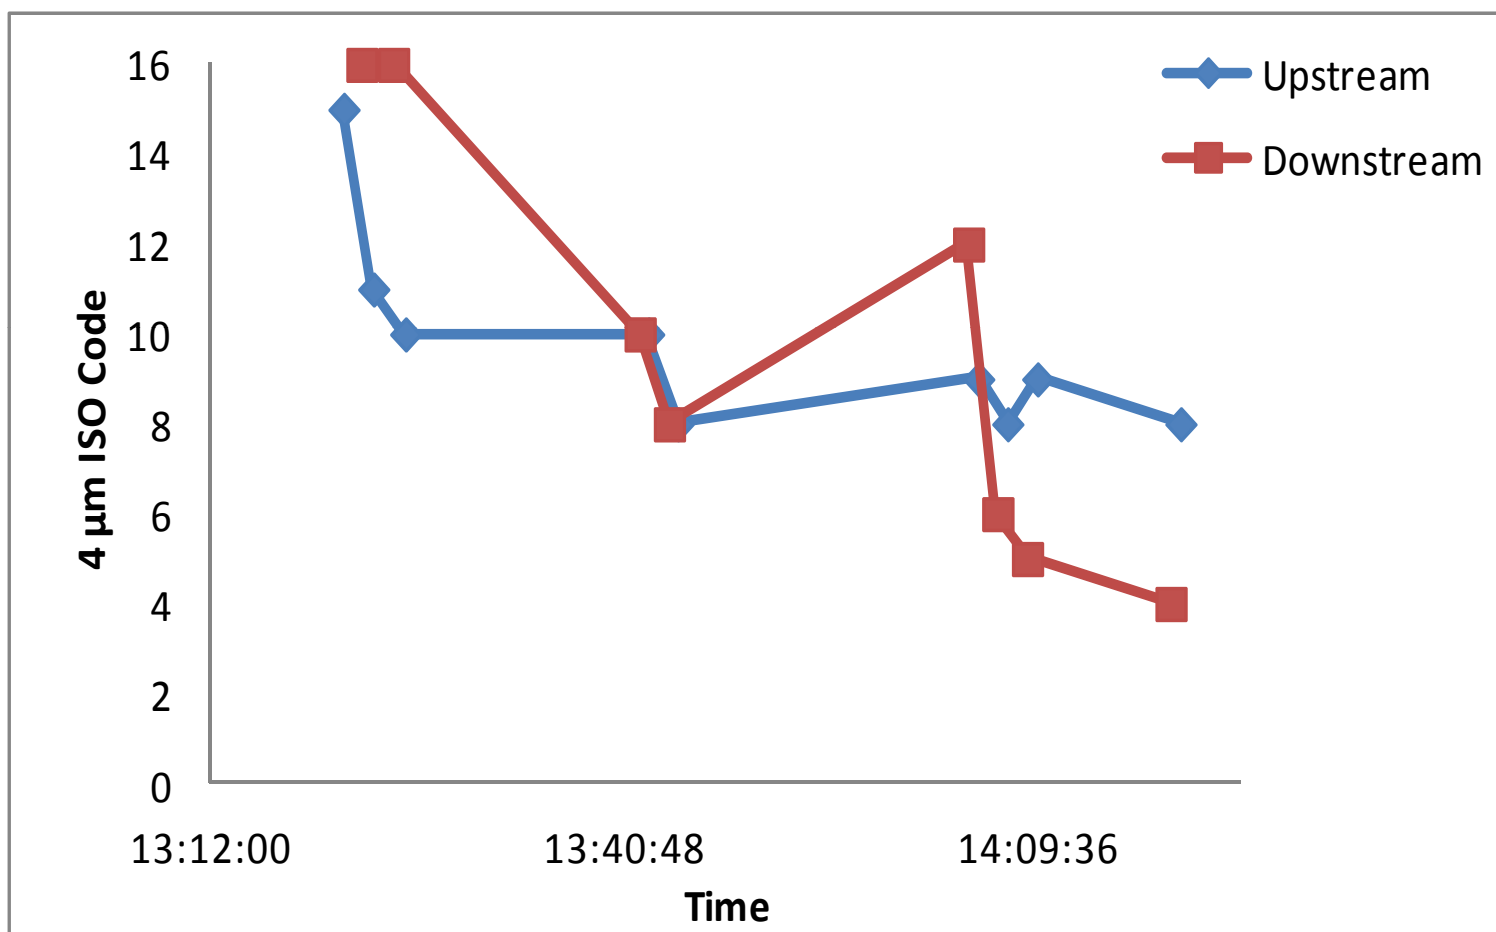



Site II – Location C Issue samples

Unclassified



Time (EST)	Location	Sample #	Avcount	ACM20	S40 AVTUR	IcountOS
1300	upstream	5	17/15/11/7	17/14/10/6	17/15/11/-	15/13/9/7
1300	downstream	4	17/15/12/7	16/15/10/5	17/15/12/-	14/12/9/7
1340	upstream	3	17/15/12/9	17/15/11/7	17/15/12/-	16/14/12/10
1340	downstream	6	15/14/11/8	15/13/10/7	15/13/11/-	-
1355	upstream	11	17/15/12/8	16/14/10/6	16/14/11/-	13/11/7/6
1355	downstream	12	16/14/11/7	16/14/10/6	16/14/11/-	11/10/5/0
1435	upstream	9	17/15/12/9	16/14/11/7	16/15/12/-	-
1435	downstream	10	18/16/14/9	17/16/12/8	18/16/14/-	14/13/11/11
1300	upstream	17	17/15/10/6	17/14/9/5	17/15/11/-	12/11/8/4
1300	downstream	18	17/15/11/6	17/14/10/6	17/15/11/-	13/11/8/6
1320	upstream	32	17/15/11/7	17/15/10/7	17/15/11/-	15/13/10/7
1320	downstream	33	17/15/11/7	16/14/10/6	17/14/11/-	16/14/12/12



Conclusions

Unclassified



- Bottle sampling has the likelihood to induce contamination into measurements that is not present in the fuel stream.
- Particle counters are affected by air bubbles in the fuel stream.
- Proposed 19/17/14/13 is an acceptable working limit.
- 92F desire to replace existing aqua-glo free water testing.



Lessons Learned

Unclassified



- AFCTK sampling apparatus and bottles leak.
- AFCTK sampling hose has the potential to induce contamination.
- Sample port valves improve fuel sample cleanliness and reduce fuel spillage.